

# BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: CSSD

## PART-I KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)

Sr. No.	Evaluation Parameters	Total Technology	Mediland Pakistan	Radiant Medical	Clinical Life	Vertex Medical	Universal Ent.
1	Complete Package/Tender	Yes	Yes	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II

*[Handwritten Signature]*  
*[Handwritten Signature]*  
*[Handwritten Signature]*

PART- II

Sr. No.	Evaluation Parameters	Total Technology	Mediland Pakistan	Radiant Medical	Clinical Life	Vertex Medical	Universal Ent.
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	Yes	Yes	Yes	Yes	Yes	No legal attested sole authorization
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes	Yes	Yes	No
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	Yes	No Satisfactory Report of washer disinfecter	Yes	No Satisfactory Report Attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes	Yes	No Warranty from the manufacturer
	Remarks:	Eligible for part III	Eligible for part III	Eligible for part III	Not Eligible for part III	Eligible for part III	Not Eligible for part III

*[Handwritten signatures and initials]*


## SPECIFICATION COMPLIANCE /EVALUATION PARAMETERS


Name of Equipment	COMPANY	Total Technology	Mediland Pakistan	Radiant Medical	Clinical Life	Vertex Medical	Universal Ent.
	Manufacturer Model	Make MMM Group	Getinge	Matachana	AJ Costa	Belimed	DGM Pharma- Apparate Handel AG
		Washer Disinfector Model: Uniclean PL-II 15-2 Heavy duty steam sterilizer: Selcetomat PL 6612-2 CL Medium Sterilizer: Selcetomat PL 666-2 CL Electronic Autoclave: Selcetomat PL 636-1 CL	Washer Disinfector Model: Getinge 8668/ Getinge Infection Control Sweden Heavy duty steam sterilizer: TS 555 EC2 NX Trans Getinge Turkey Medium Sterilizer: TS 330 EC 2NX Trans Getinge Turkey Electronic Autoclave: HS33 Getinge Infection Control Sweden	Washer Disinfector Model: MAT LD 1000 M- 2 Ken Denmark supplied by Matachana Spain Heavy duty steam sterilizer: S1008 E-2, Matachana Spain	Washer Disinfector Model: IQ6 Ken Denmark supplied by AJ Costa Portugal Heavy duty steam sterilizer: Amaro 5000 AJC 7070125-2D GI AJ Costa Portugal Medium Sterilizer: Amaro 5000 AJC 707070-2D GI AJ Costa Portugal Electronic Autoclave: Steri 21 AJC 4040466- 1D GI AJ Costa Portugal	Washer Disinfector Model: WD-290 Heavy duty steam sterilizer: MST- V6-6-12 Medium Sterilizer: MST-V6-6-6 VS2 Electronic Autoclave: Vapofix 3-3-9 Belimed	Washer Disinfector Model: DGM ES-350P Heavy Duty sterilizer: DMG ANDS-600/2 Medium Sterilizer: DMG ANDS-300/2 Electronic Autoclave: DMG ANDS-100/1 DGM Pharma- Apparate Handel AG Switzerland
Country of Manufacturer	Germany	Sweden	Spain	Portugal	Switzerland	Switzerland	
Country of Origin of Product/Model Number	Germany	As mentioned above	As mentioned above	As mentioned above	Slovenia	Switzerland	
Compliance with defined quality standards	Yes	Yes	Yes	Yes	Yes	Yes	
Specification Compliance features wise:							

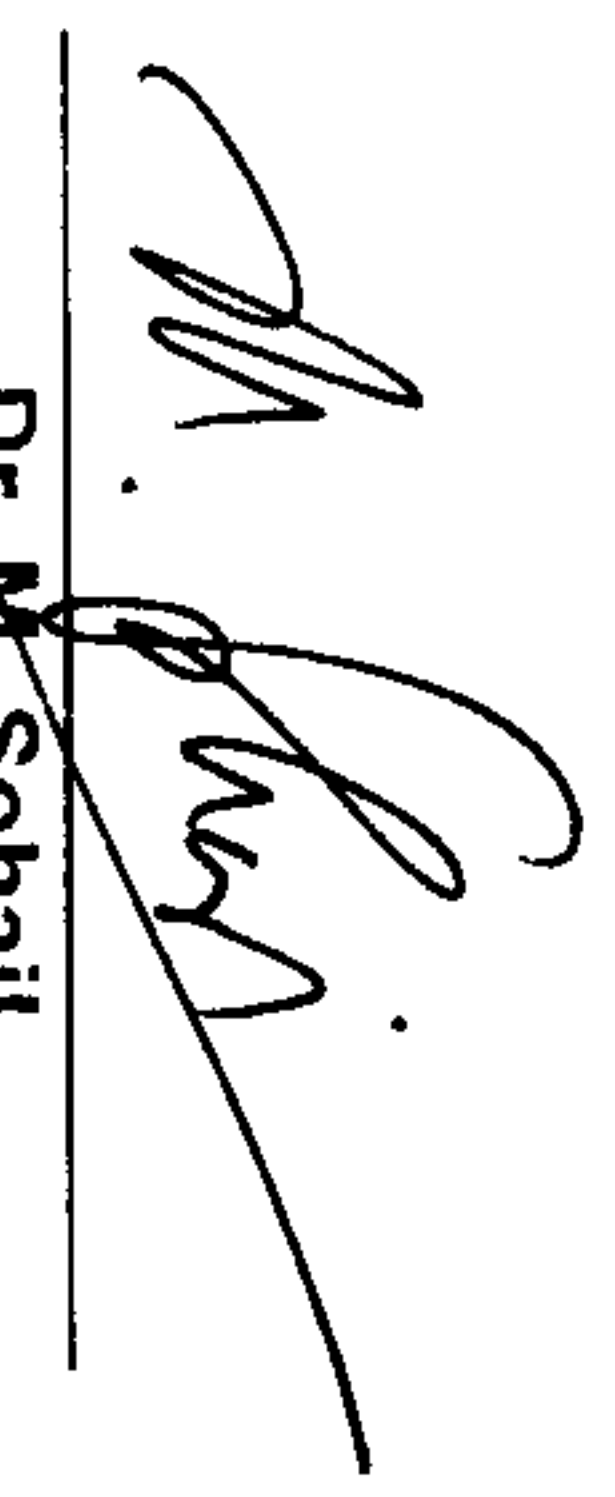
Handwritten signature and initials, possibly 'D.M.' and 'D.P.', with a large flourish.


10/19

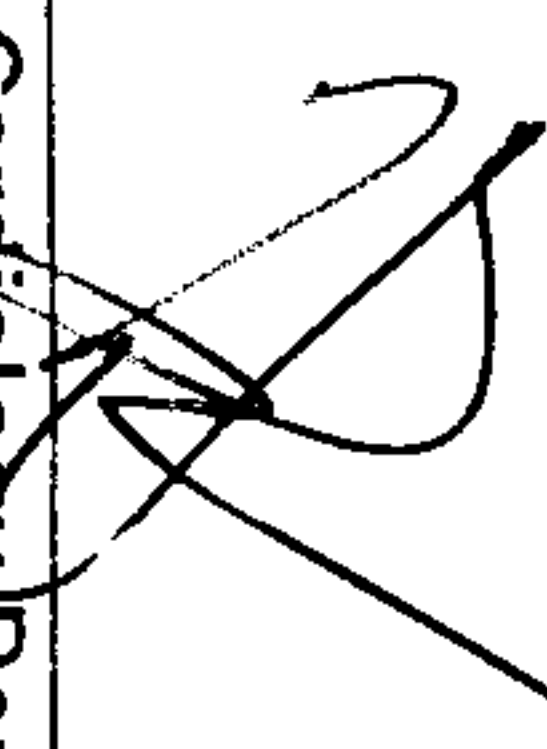
Specifications:	Yes	Yes	Yes	No Medium sterilizer model available on manufacturer website	Heavy, medium & electronic steam sterilizer have touchpad screen instead of color touch screen	Washer disinfector No touch screen Vertical upward sliding doors instead of vertical downward sliding doors MIS instrument, instrument trays, Rack for 25 shoes pair and transfer trolleys are quoted as optional instead of standard UPS not offered for heavy, medium & electronic steam sterilizer 1 loading cart offered instead of 2 for heavy duty steam sterilizer Transport and distribution trolleys model not mentioned furthermore country of manufacturer not as required CSSD renovation not offered
Technical Eligibility of Product:	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Not Eligible
Technical Eligibility of Firm:	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Not Eligible
BID STATUS:	Responsive	Responsive	Responsive	Non Responsive	Non Responsive	Non Responsive

  
**Mr. Haseeb Aslam**  
 BioMedical Engineer  
 Nominated by SHC&ME Department, Lahore  
 (Member)

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
 (Member)

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
 (Member)

  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
 (Chairman)

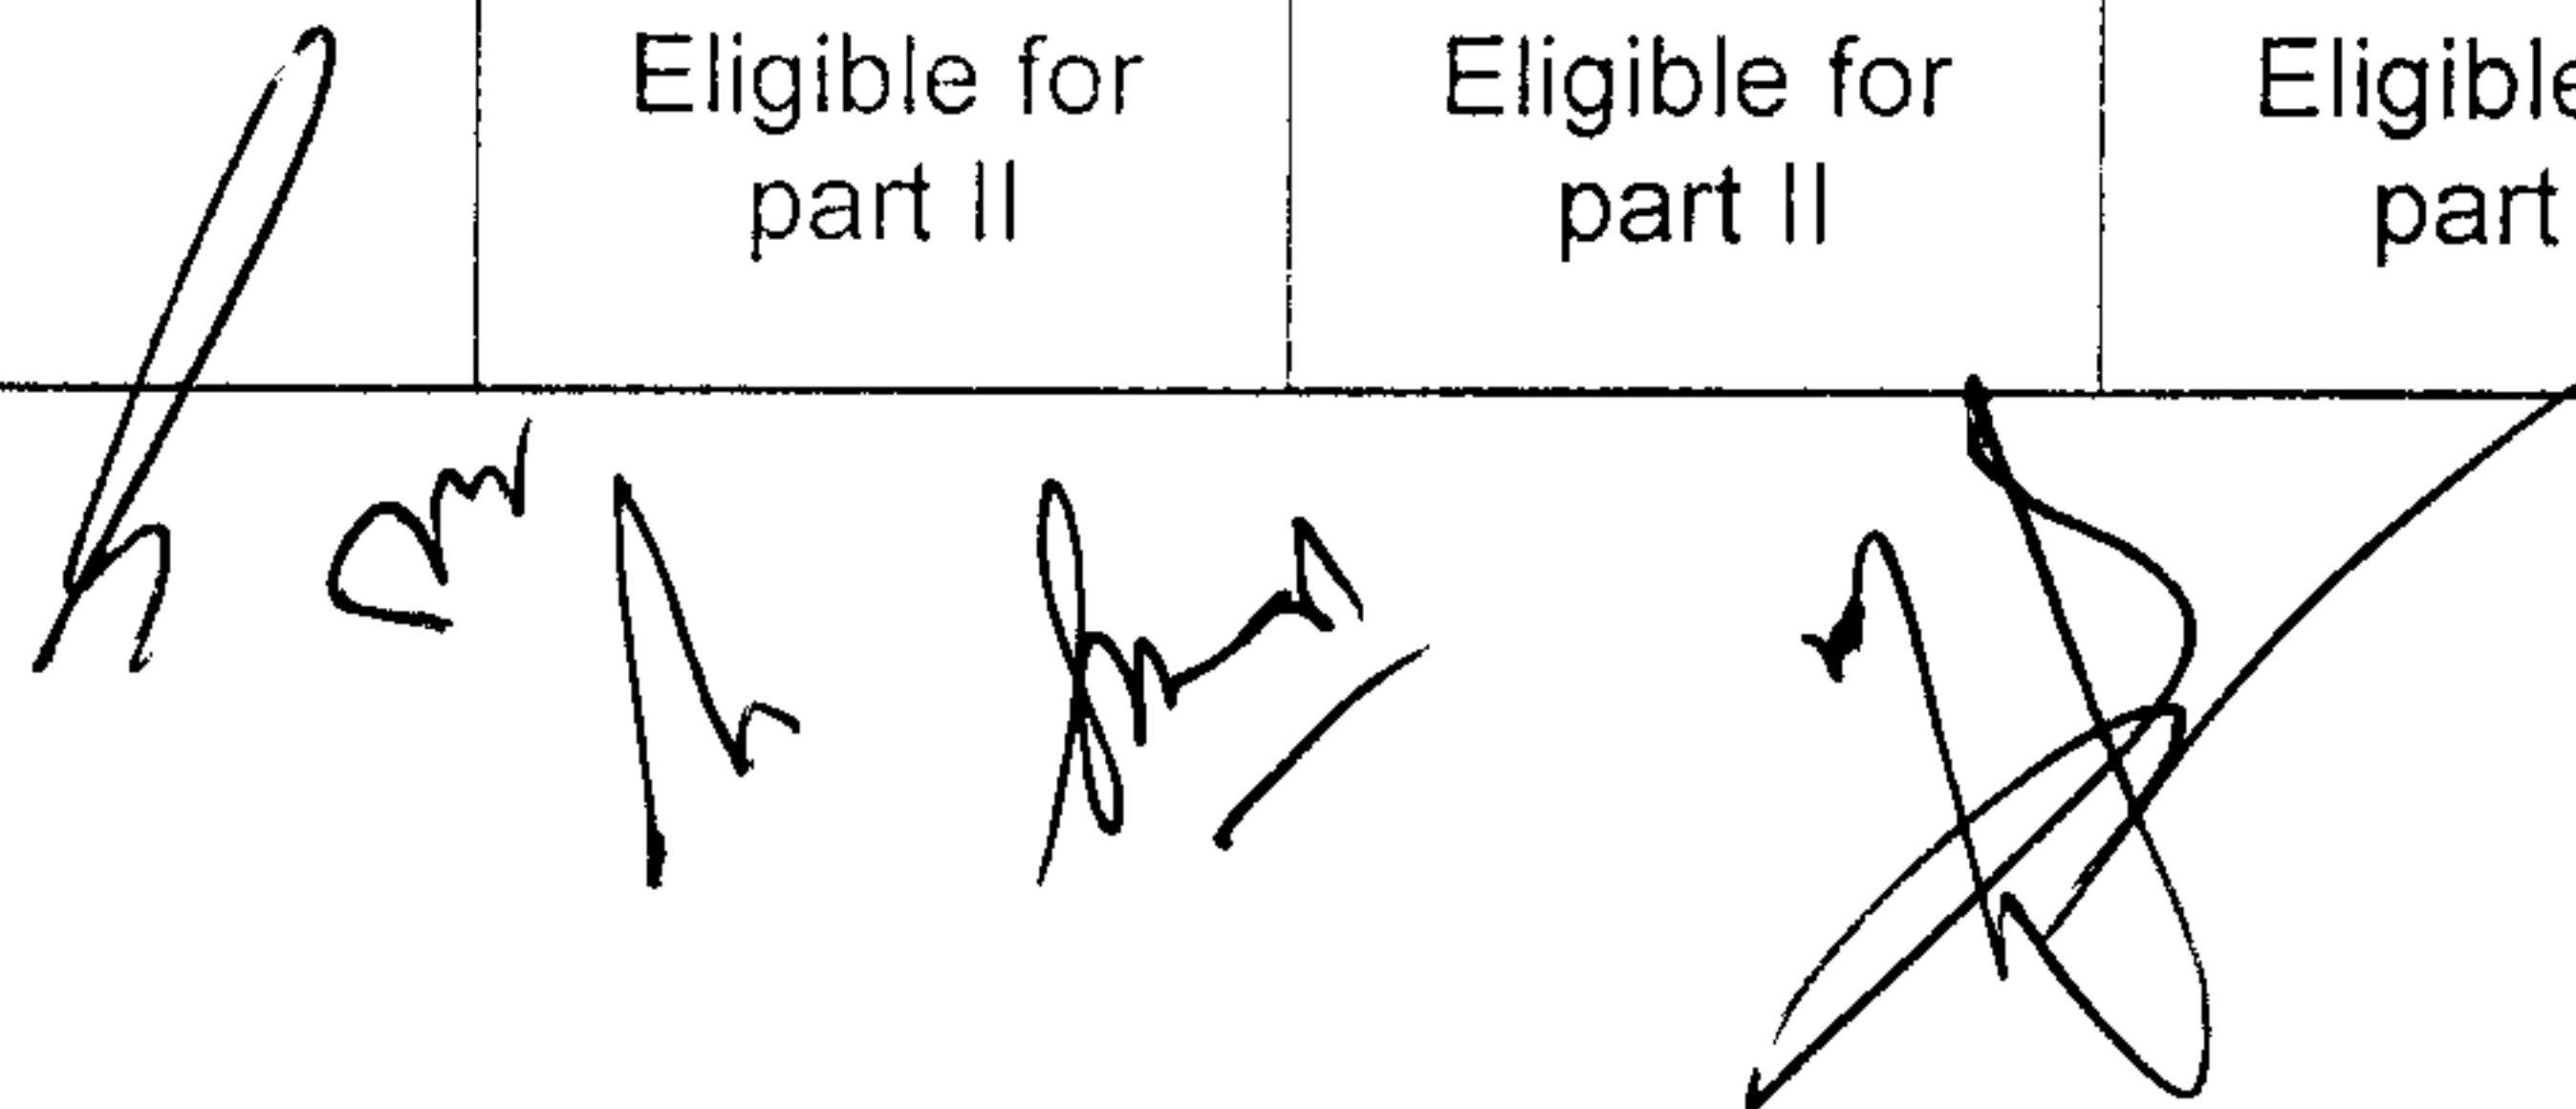
## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: STERNUM SAW

**PART- I**

**KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Claris Medical	Kasbn Int.	Vertex Medical	Universal Enterprises
1	Complete Package/Tender	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II




PART- II


Sr. No.	Evaluation Parameters	Claris Medical	Kasbn Int.	Vertex Medical	Universal Enterprises
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	No Embassy Attested Authorization	Yes	Yes	Yes
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes	Yes
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	No Sale reference/ satisfactory report attached	Yes	No Satisfactory report attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes
	Remarks:	Not Eligible for part III	Not Eligible for part III	Eligible for part III	Not Eligible for part III

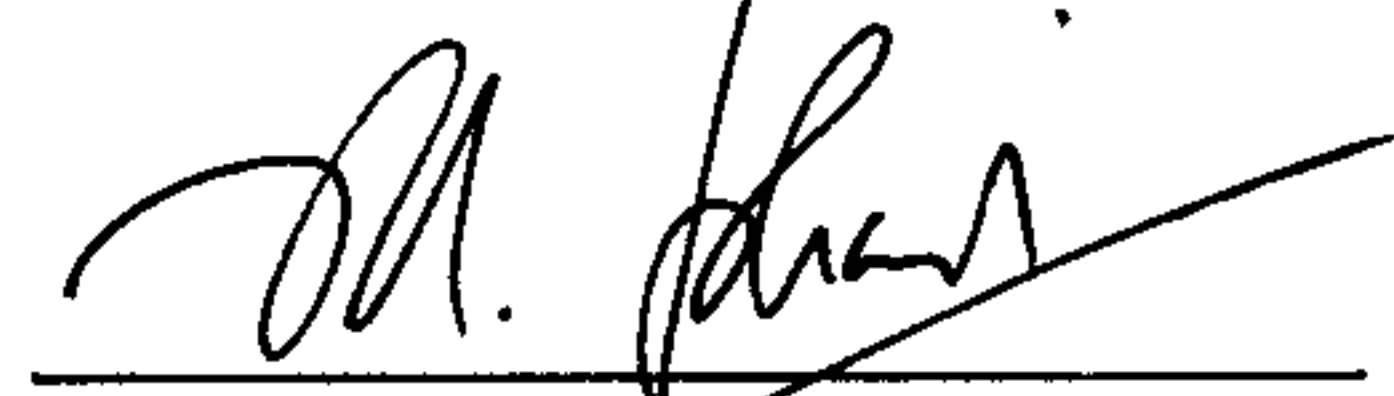
*[Handwritten signatures and initials are present below the table, including a large signature on the left and several smaller ones below it.]*


PART – III


Name of Equipment	COMPANY	Clariss Medical	Kasbn Int.	Vertex Medical	Universal Enterprises
Sternum Saw	Manufacturer	Desoutter Medical	Nouvag AG	B-Braun Aesulap AG	Tekno MBS
	Model	DBC 470	3704	Acculan 4 GA 334	3360
Country of Manufacturer		UK	Switzerland	Germany	Germany
Country of Origin of Product/Model Number		UK	Switzerland	Germany	Germany
Compliance with defined quality standards		Yes	No No CE for sternum saw as per listed scope on attached certificate	Yes	Yes
Specification Compliance features wise:					
Specifications:		No Blade quoted 200 instead of 600		Yes	No Quoted unit is desktop electric instead of handy battery operated
Technical Eligibility of Product:		Not Eligible	Not Eligible	Eligible	Not Eligible
Technical Eligibility of Firm:		Not Eligible	Not Eligible	Eligible	Not Eligible
BID STATUS:		Non Responsive	Non Responsive	Responsive	Non Responsive

  
**Mr. Haseeb Aslam**  
**BioMedical Engineer**  
 Nominated by SHC&ME Department,  
 Lahore  
**(Member)**

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
**(Member)**

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
**(Member)**

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
**(Member)**

  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
**(Chairman)**

**BID EVALUATION SHEET/TECHNICAL SHEET**  
**NAME OF THE EQUIPMENT: ANESTHESIA MACHINE (1B)**

**PART-I**  
**KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading	Clinical Life
1	Complete Package/Tender	Yes	Yes	Yes	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II

*Handwritten signatures and initials:*  
 PE [Signature] [Signature] [Signature]



PART- II

Sr. No.	Evaluation Parameters	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading	Clinical Life
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	No legal attested sole authorization	No legal attested sole authorization	Yes	Yes	Yes	Yes	Yes
2	Technical & Engineering capability/As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	N/A	N/A	N/A	N/A	N/A	N/A	N/A
4	Vendor Past performance (in case of unsatisfactory performance, details must be mentioned)	No sale reference/ satisfactory report from end-user	No sale reference/ satisfactory report from end-user	Yes	Yes	Yes	Yes	Yes
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	Remarks:	Not Eligible for part III	Not Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III

*Handwritten signature*

*cm*

*Handwritten signature*

*Handwritten signature*

PART - III

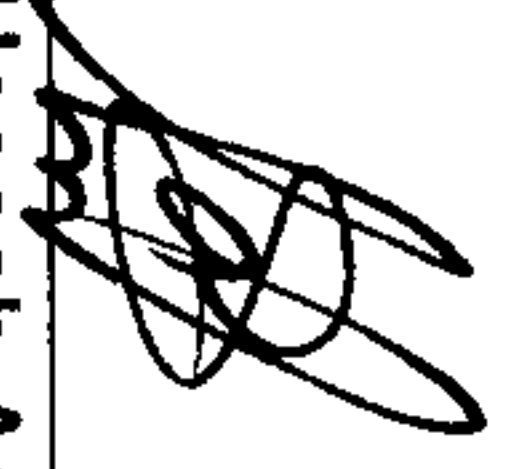
SPECIFICATION COMPLIANCE /EVALUATION PARAMETERS

Name of Equipment	COMPANY	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading	Clinical Life
<u>Anesthesia Machine</u> (1B)	Manufacturer	Oricare	Siare	Dragwerk	Dameca	Penlon	GE Healthcare	Chirana.S
	Model	A9800, Monitor Model: M-7810	Morpheus/E-Light Monitor Model: 2000PPM advanced USA	Primus Monitor Model: IACS C500	AX-700 Monitor Model: Intellivue MX-800 Philips USA	Prima 465 Monitor Model: SP M8	Advance CS2 Monitor Model: B125	Venar TS Monitor Model: XL189
Country of Manufacturer	USA	Italy	Germany	Denmark	UK	USA	Slovakia	
Country of Origin of Product/Model Number	China	Italy	Germany	Denmark	UK	China	Slovakia	
Compliance with defined quality standards	Yes	Yes	Yes	Yes	Yes	Yes	Yes	
Specification Compliance features wise:								
Specifications:	No Tidal volume started from 20ml instead of 5ml	No Cardiac Bypass Mode not offered, quoted monitor is not compatible with the machine quoted monitor is not from the same manufacturer, no electronic mixing, cylinder gauge is not available, power outlets with sockets only 1 instead of 3-4, scavenging system is not available	Yes	No Tidal volume started from 20ml instead of 5ml No SIMV with PS mode No integrated heating system PEEP min value is 4 instead of 3	Demo unit not provided	Yes	Yes	

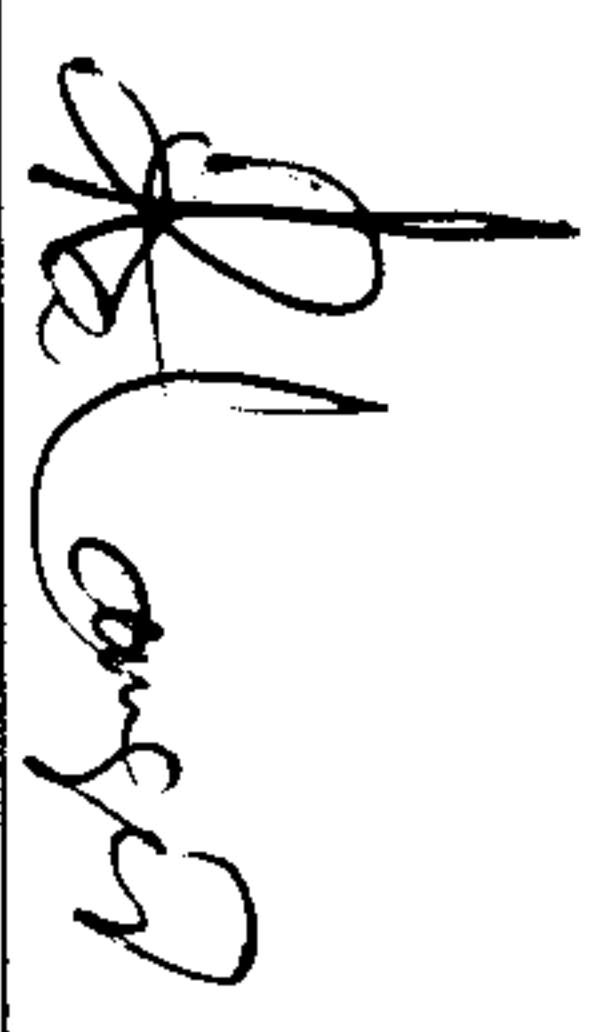
*Handwritten signatures and initials:*  
 A large signature resembling "SR" is written across the middle of the table.  
 Other initials "ML" and "M" are visible on the left side.

*Anesthetics*

Technical Eligibility of Product:	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Eligible	Eligible
Technical Eligibility of Firm:	Not Eligible	Not Eligible	Eligible	Eligible	Eligible	Eligible	Eligible
BID STATUS:	Non Responsive	Non Responsive	Responsive	Non Responsive	Non Responsive	Responsive	Responsive



Mr. Haseeb Aslam  
BioMedical Engineer  
Nominated by SHC&ME Department, Lahore  
(Member)



Dr. Asif Rashid Alamgir  
Consultant Anesthetist  
(Copt. Member)

*CMV*

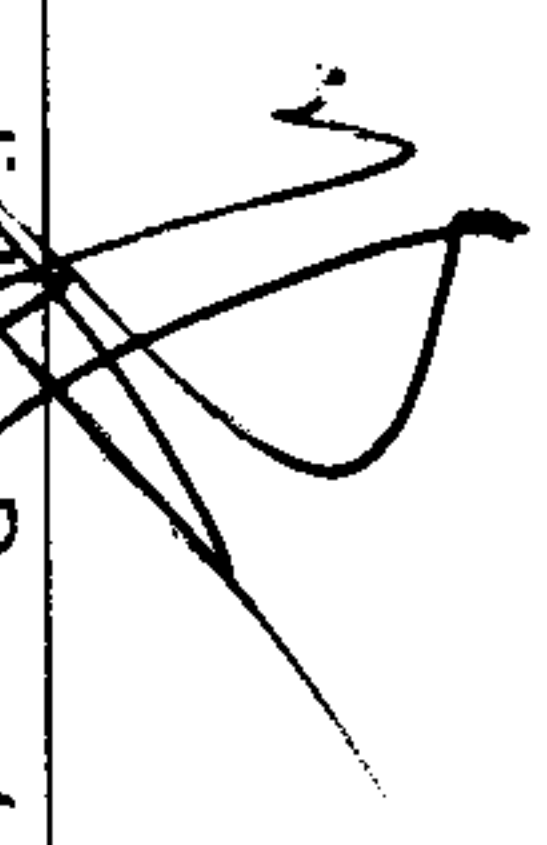
Electronic Equipment Care Taker  
F.I.C. Faisalabad  
(Member)



Dr. M. Sohail  
Assistant Prof. Cardiac Surgery  
F.I.C. Faisalabad  
(Member)



ANMS (P&D)  
F.I.C. Faisalabad  
(Member)



Head of Cardiology Department  
F.I.C. Faisalabad  
(Chairman)

**BID EVALUATION SHEET/TECHNICAL SHEET**  
**NAME OF THE EQUIPMENT: ANESTHESIA MACHINE (1A)**


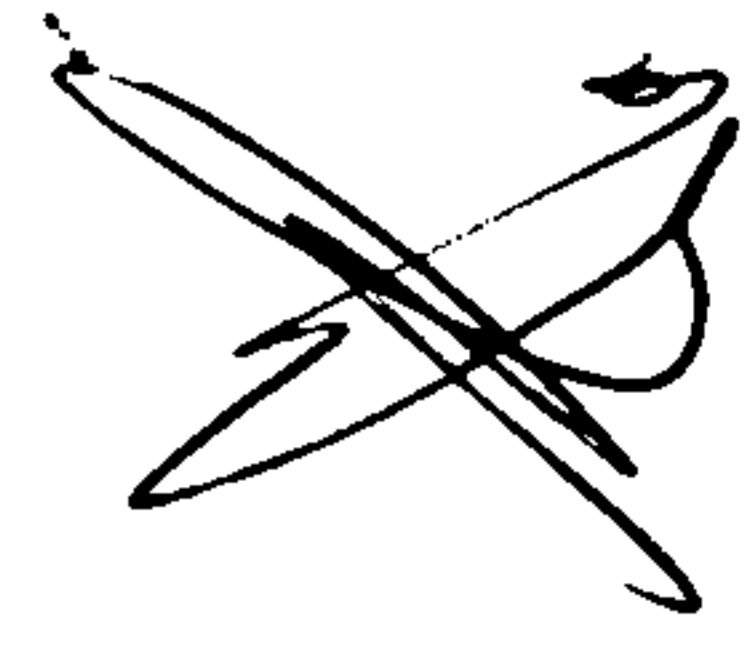



**PART-I**  
**KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading
1	Complete Package/Tender	Yes	Yes	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part III	Eligible for part II

*PK* *[Signature]* *M* *DM* *[Signature]*

PART-II

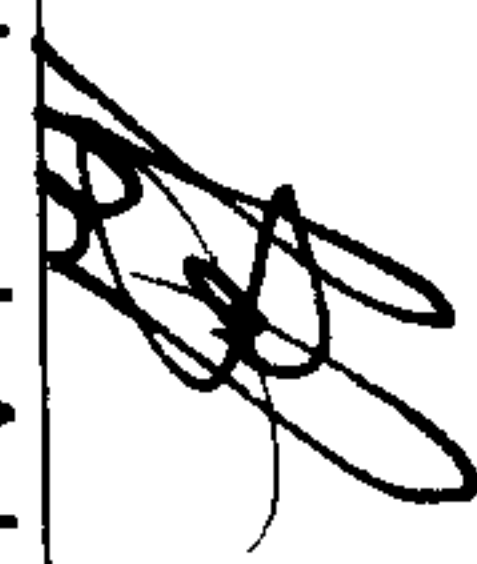
Sr. No.	Evaluation Parameters	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	No legal attested sole authorization	No legal attested sole authorization	Yes	Yes	Yes	Yes
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	N/A	N/A	N/A	N/A	N/A	N/A
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	No sale reference/ satisfactory report from end-user	No sale reference/ satisfactory report from end-user	Yes	Yes	Yes	Yes
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Warranty of batteries, O2 sensor and flow sensor not offered	Yes	Yes	Yes	Yes
	Remarks:	Not Eligible for part III	Not Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III









PART - III


SPECIFICATION COMPLIANCE /EVALUATION PARAMETERS


Name of Equipment	COMPANY	Medi Bridge	Eastern Medical	Vertex Medical	Radiant Medical	Digonics	Sherazi Trading
Anesthesia Machine (1A)	Manufacturer	Oricare	Siare	Dragwerk	Dameca	Penlon	GE Healthcare
	Model	A9800, Monitor Model: M-7610	Morpheus/M-Light Monitor Model: Neptune 12" TS	Fabius Plus Monitor Model: Vista-120 China	AX-500 Monitor Model: Efficia CM-12 Philips	Prima 450 Monitor Model: SP M5	9100c NXT Monitor Model: B125
Country of Manufacturer		USA	Italy	Germany	Denmark	UK	USA
Country of Origin of Product/Model Number		China	Italy	China	Denmark	UK	China
Compliance with defined quality standards		Yes	Yes	Yes	Yes	Yes	Yes
Specification Compliance features wise:							
Specifications:		No virtual tubes of flow meter	Absorber support bag not offered	Yes	Yes	Yes	Yes
Technical Eligibility of Product:		Not Eligible	Not Eligible	Eligible	Eligible	Eligible	Eligible
Technical Eligibility of Firm:		Not Eligible	Not Eligible	Eligible	Eligible	Eligible	Eligible
BID STATUS:		Non Responsive	Non Responsive	Responsive	Responsive	Responsive	Responsive

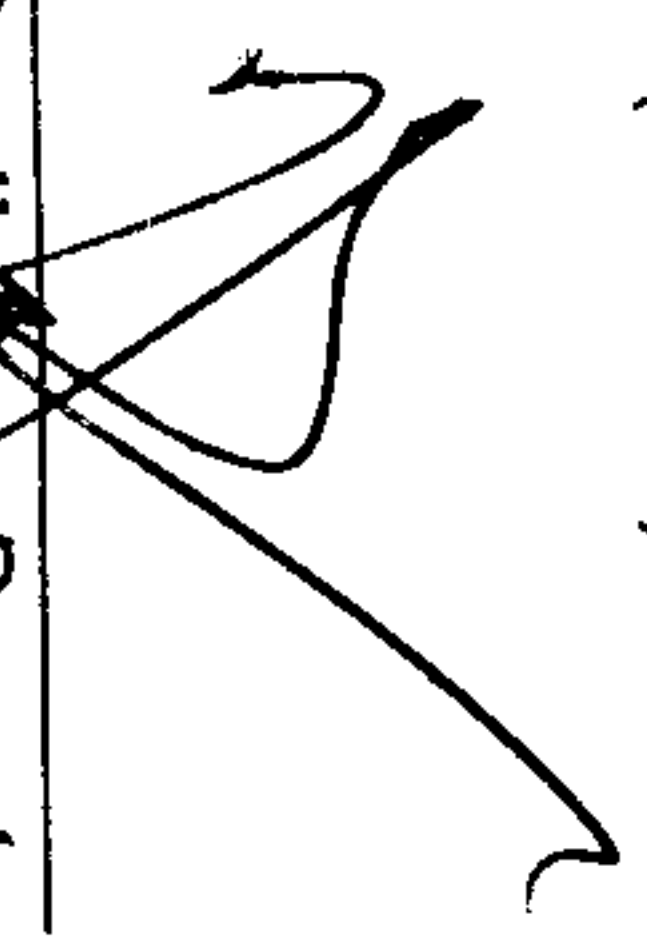
  
**Mr. Haseeb Aslam**  
 BioMedical Engineer  
 Nominated by SHC&ME Department, Lahore  
 (Member)

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
**Dr. Asif Rashid Alamgir**  
 Consultant Anesthetist  
 (Copt. Member)

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
 (Member)

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
 (Member)

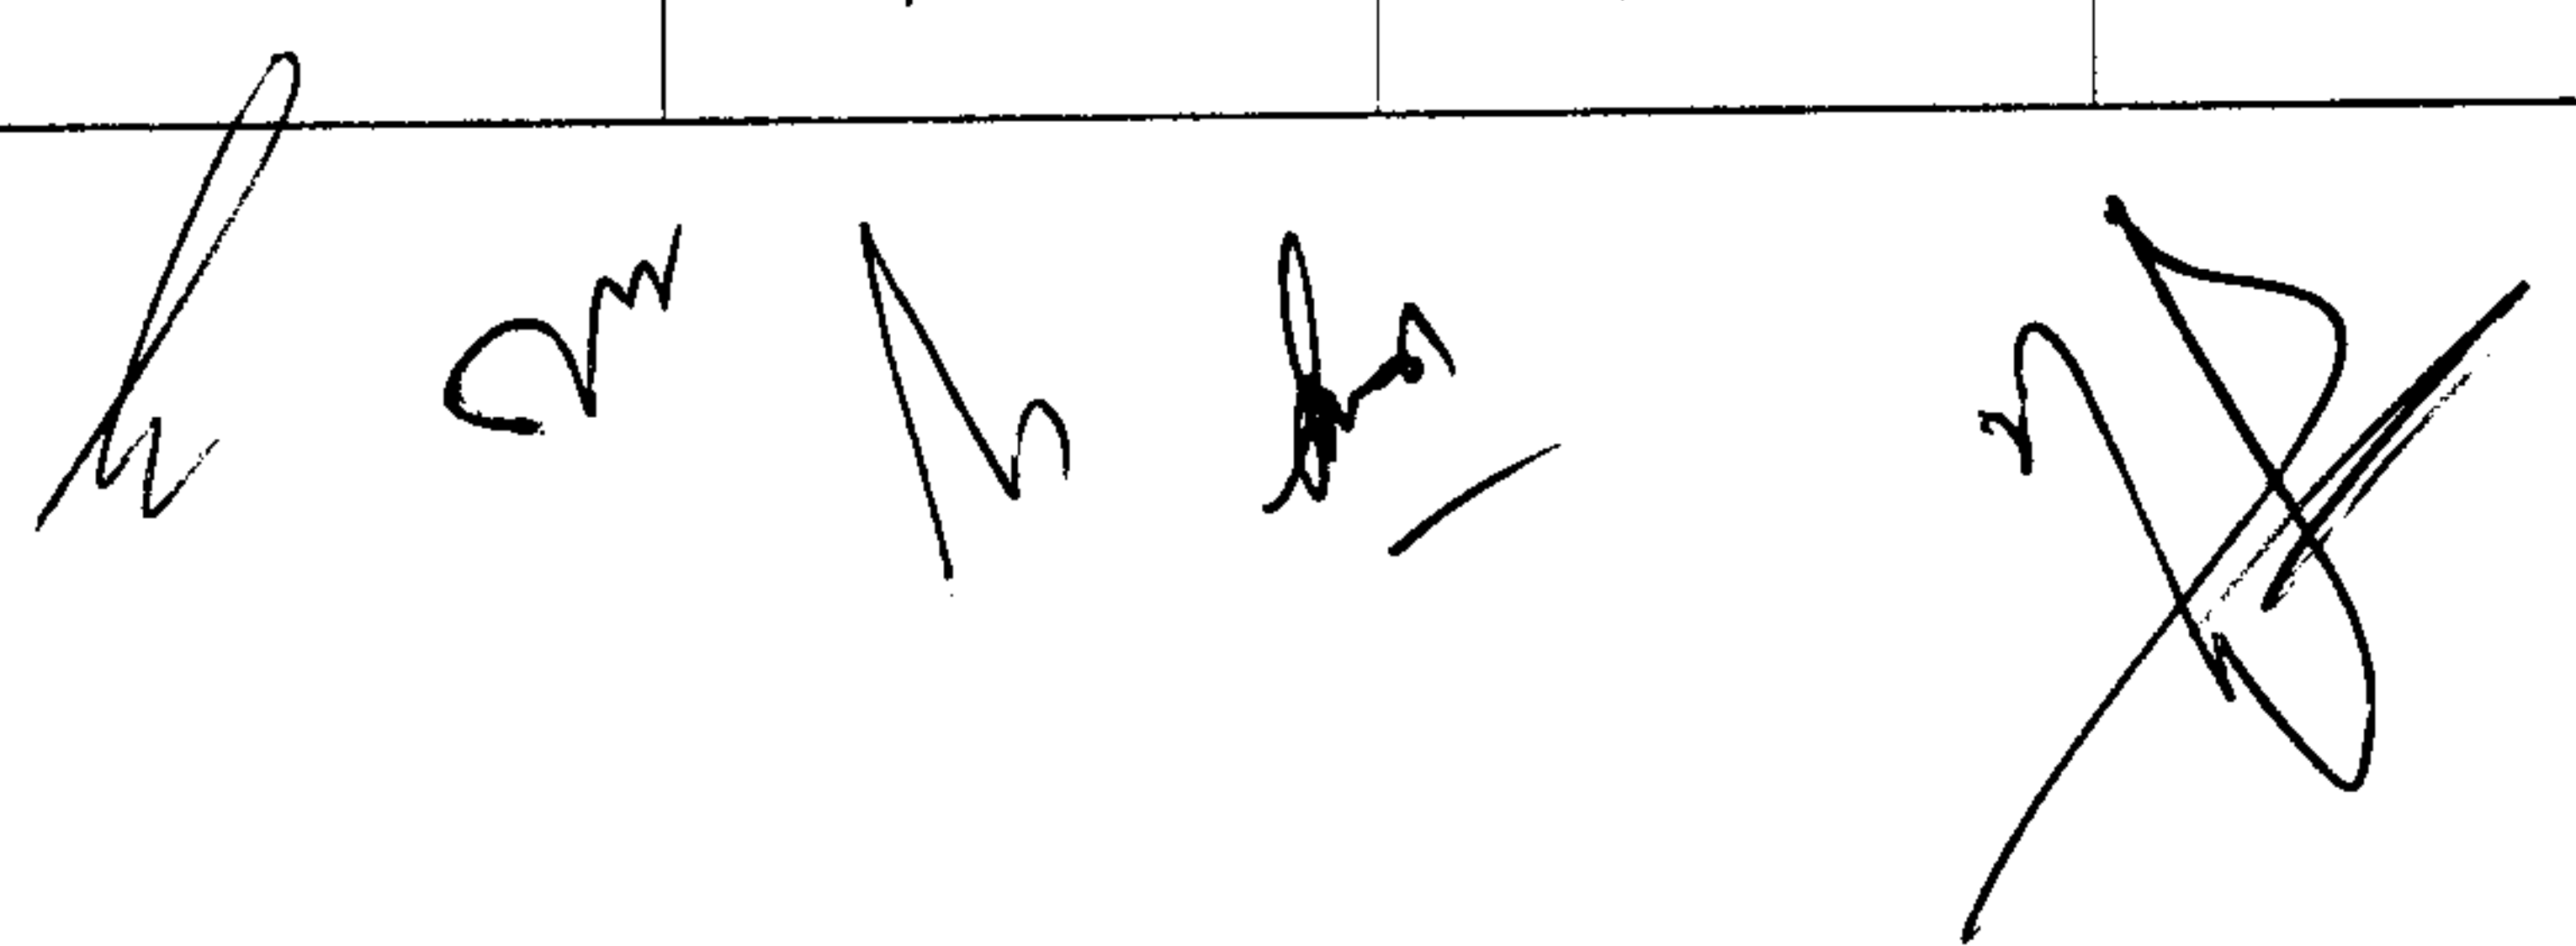
  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
 (Chairman)

## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: HEART LUNG MACHINE

**PART- I**  
**KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Universal Ent.	Mediland Pakistan	Medica	Medtronic
1	Complete Package/Tender	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II



PART- II

Sr. No.	Evaluation Parameters	Universal Ent.	Mediland Pakistan	Medica	Medtronic
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	No Embassy Attested Authorization	Yes	Yes	Yes
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	No	Yes	Yes	Yes
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	Yes	No Satisfactory report attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	No 5 years warranty from the manufacturer not provided	Yes	Yes	Yes
	Remarks:	Not Eligible for part III	Eligible for part III	Eligible for part III	Not Eligible for part III


*Handwritten signature/initials*


*Handwritten signature*

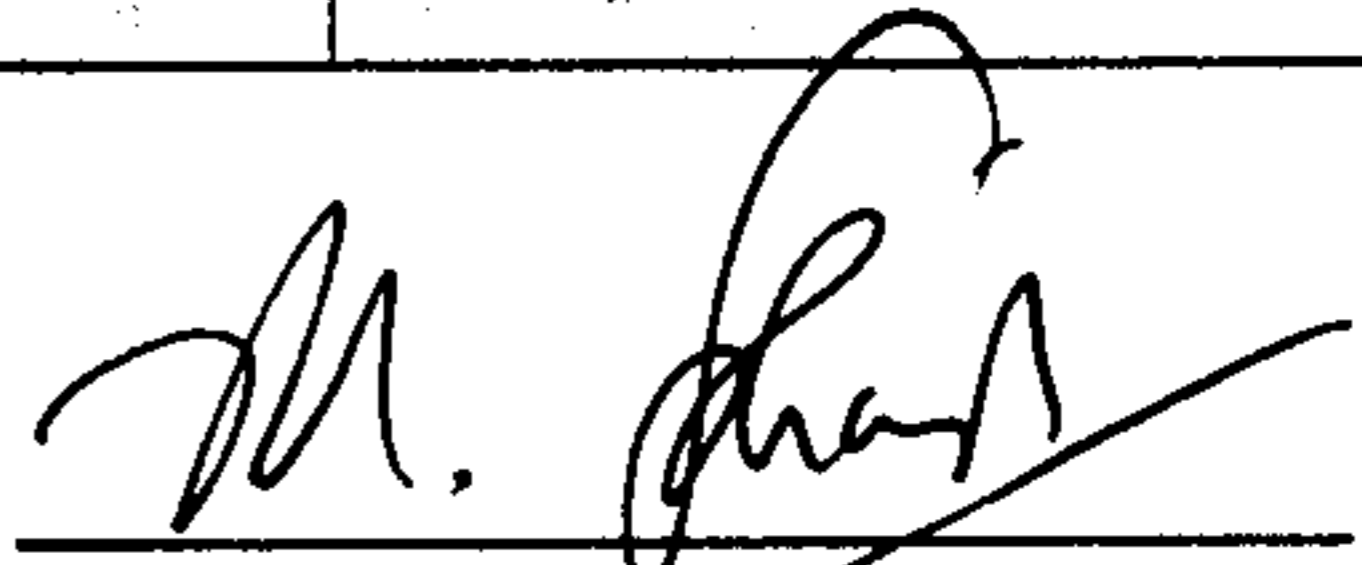



**PART – III**


Name of Equipment	COMPANY	Universal Ent.	Mediland Pakistan	Medica	Medtronic
Heart Lung Machine	Manufacturer	Terumo	Getinge Group	Sorin Liva Nova	Spectrum Medical
	Model	Advance perfusion system 1 Optional Monitor Model: CDI550 USA Japan	HL20 vario twin Optional Monitor Model: BMU 40 Getinge Group Germany	S5 Optional Monitor Model: Not offered	Diagnostic module Optional Monitor Model: Built-in
Country of Manufacturer		USA	Germany	Germany	UK
Country of Origin of Product/Model Number		Japan	Germany	Germany	UK
Compliance with defined quality standards		Yes	Yes	Yes	Yes
<b>Specification Compliance features wise:</b>					
Specifications:	No Hand crank offered 02 instead of 10 Nos. Level sensor pads offered 60 instead of 200 Nos. Two pressure offered instead of four Cardioplegia monitoring Unit not offered Halogen lamp offered instead of LED	Yes	After calculation battery backup on full load (1000 Watts) will be only 8 mins as per attached catalog 1, page # 38&39 whereas required backup is 90mins on full load Optional monitor not offered	Flexible LED lamp not offered Mechanical/electronic gas blender not offered Venous occluding clamp not mentioned in offer Hand crank for each pump not offered pulsatile mode of each roller pump is not mentioned in catalog and offer 2 pressure channel offered instead of 4 with each machine Level sensor pads not offered Standard accessories detail not mentioned in offer	
Technical Eligibility of Product:	Not Eligible	Eligible	Not Eligible	Not Eligible	
Technical Eligibility of Firm:	Not Eligible	Eligible	Eligible	Not Eligible	
<b>BID STATUS:</b>	<b>Non Responsive</b>	<b>Responsive</b>	<b>Non Responsive</b>	<b>Non Responsive</b>	

  
**Mr. Haseeb Aslam**  
**BioMedical Engineer**  
 Nominated by SHC&ME Department,  
 Lahore  
**(Member)**

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
**(Member)**

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
**(Member)**

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
**(Member)**

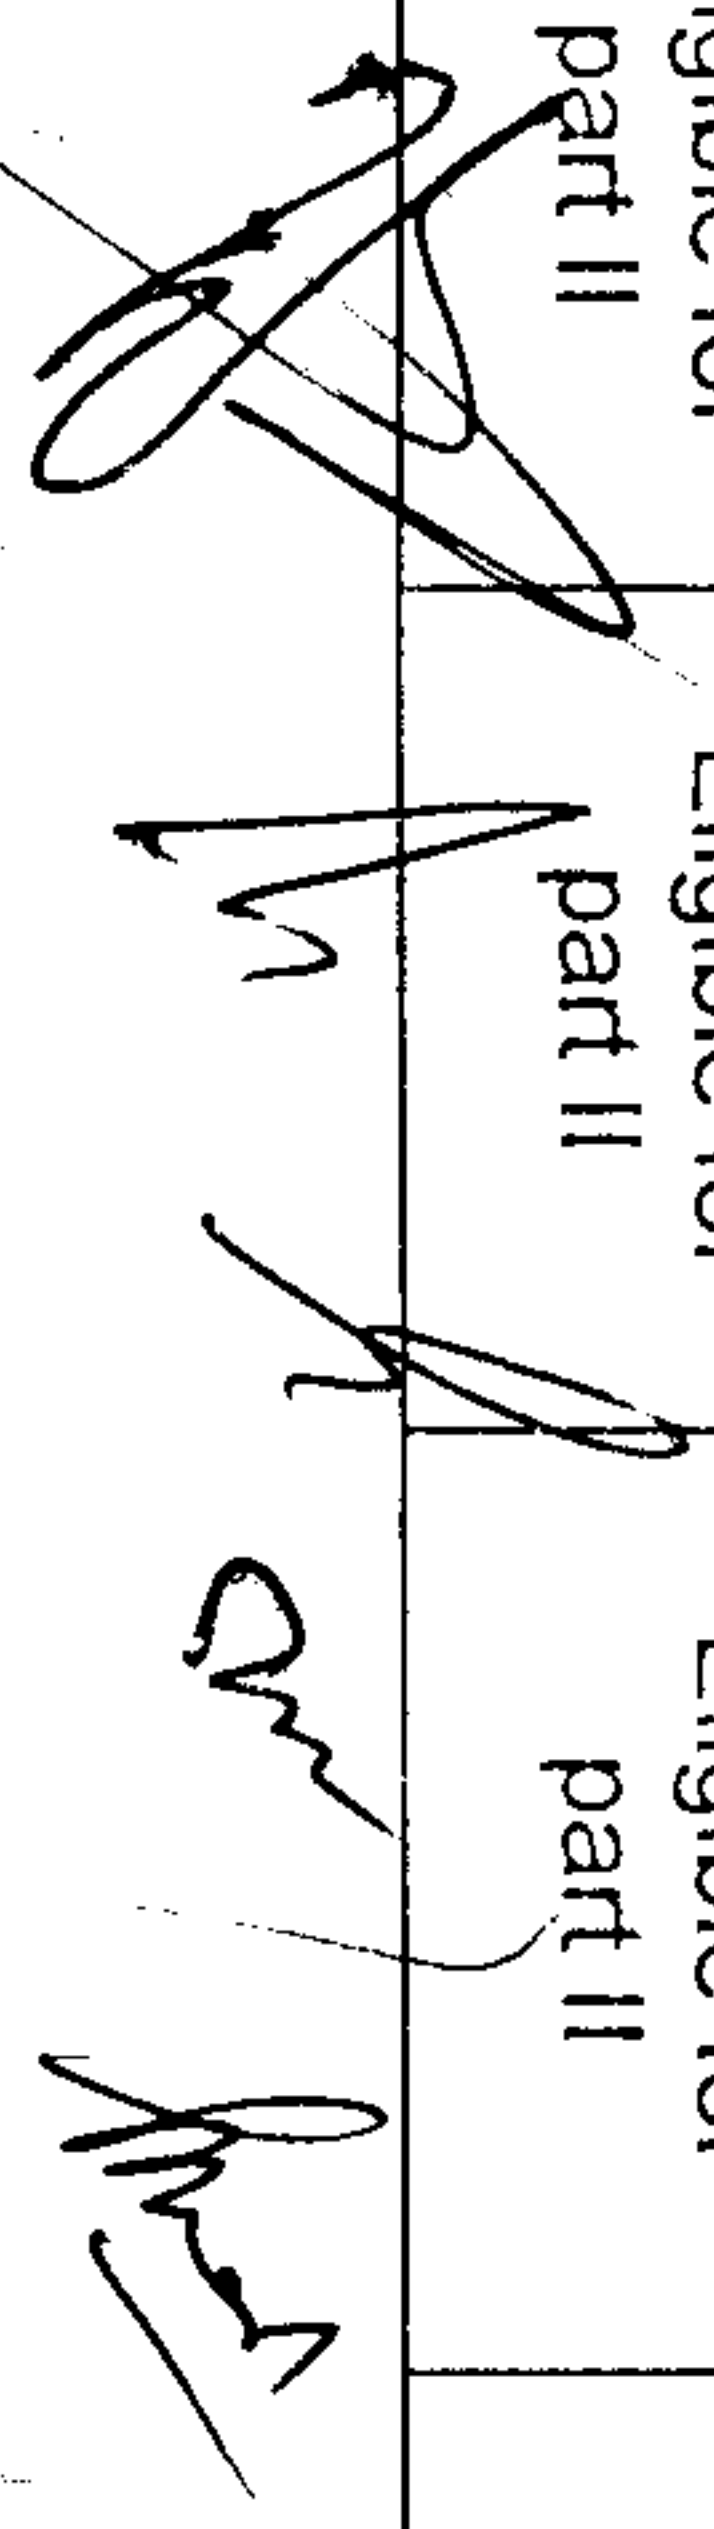
  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
**(Chairman)**

## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: Cardiac Monitor (3A)

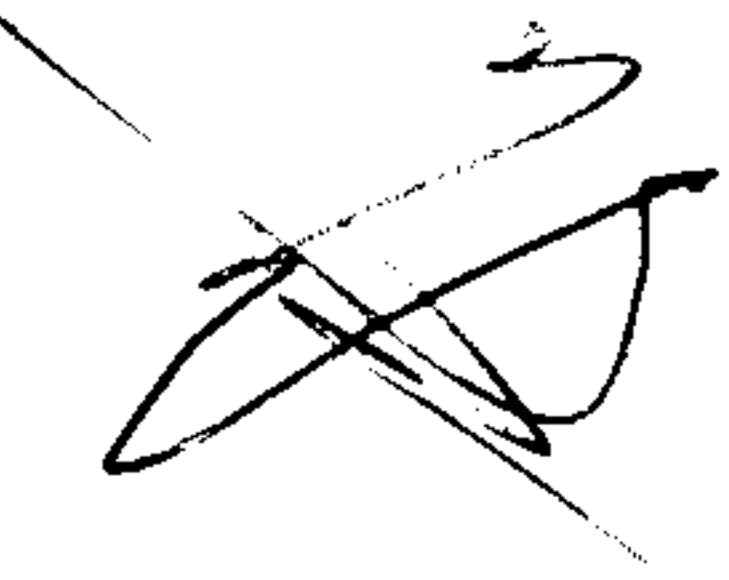


### PART-I KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)

Sr. No.	Evaluation Parameters	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron
1	Complete Package/Tender	Yes	Yes	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II



PART- II

Sr. No.	Evaluation Parameters	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	Yes	Yes	Yes	Yes	No legal attested sole authorization	No legal attested sole authorization
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes	Yes	No Technical trained engineers
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes	Yes	Yes	No
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	Yes	Yes	Yes	No Satisfactory Report Attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes	Yes	Yes
	Remarks:	Eligible for part III	Not Eligible for part III	Eligible for part III	Eligible for part III	Not Eligible for part III	Not Eligible for part III

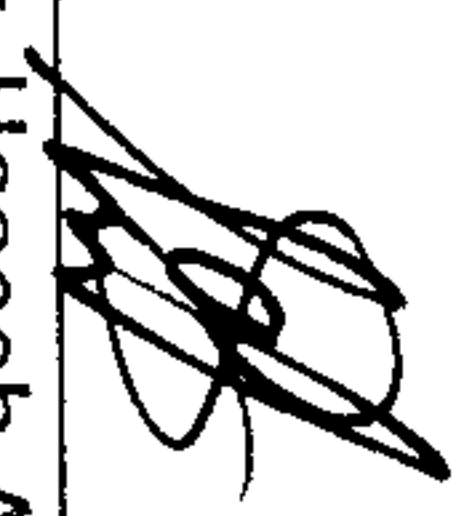
  


SPECIFICATION COMPLIANCE /EVALUATION PARAMETERS


Name of Equipment	COMPANY	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron
Cardiac Monitor (3A)	Manufacturer	Edan Instrument	Mindray	Philips	Nihon Kohden	Biolight	SpaceLab
	Model	Elite V8	Benevision N17	Intellivue MX800	Lifescop-G9 (CSM-1901)	A8	Series Exprezzon
Country of Manufacturer		China	China	USA	Japan	China	USA
Country of Origin of Product/Model Number		China	China	Germany	Japan	China	USA
Compliance with defined quality standards			Yes	Yes	Yes		No FDA 510K & CE
Specification Compliance features wise:							
Specifications:		Monitor is not intended for pediatric patients arrhythmia and ST Analysis as clearly mentioned on FDA 510K summary There are different Module models of same parameters with different specification mentioned in catalog whereas firm didn't mentioned specific model in technical offer	Yes	Yes	No External battery backup offered Local made wall mount offered	No Monitor is not intended for pediatric patients arrhythmia and ST Analysis as clearly mentioned on FDA 510K summary	No External battery backup (UPS) offered Attached FDA 510 K is for model 91393 whereas quoted model is different CE Declaration attached instead of CE Certificate from 3 <sup>rd</sup> party notifying body

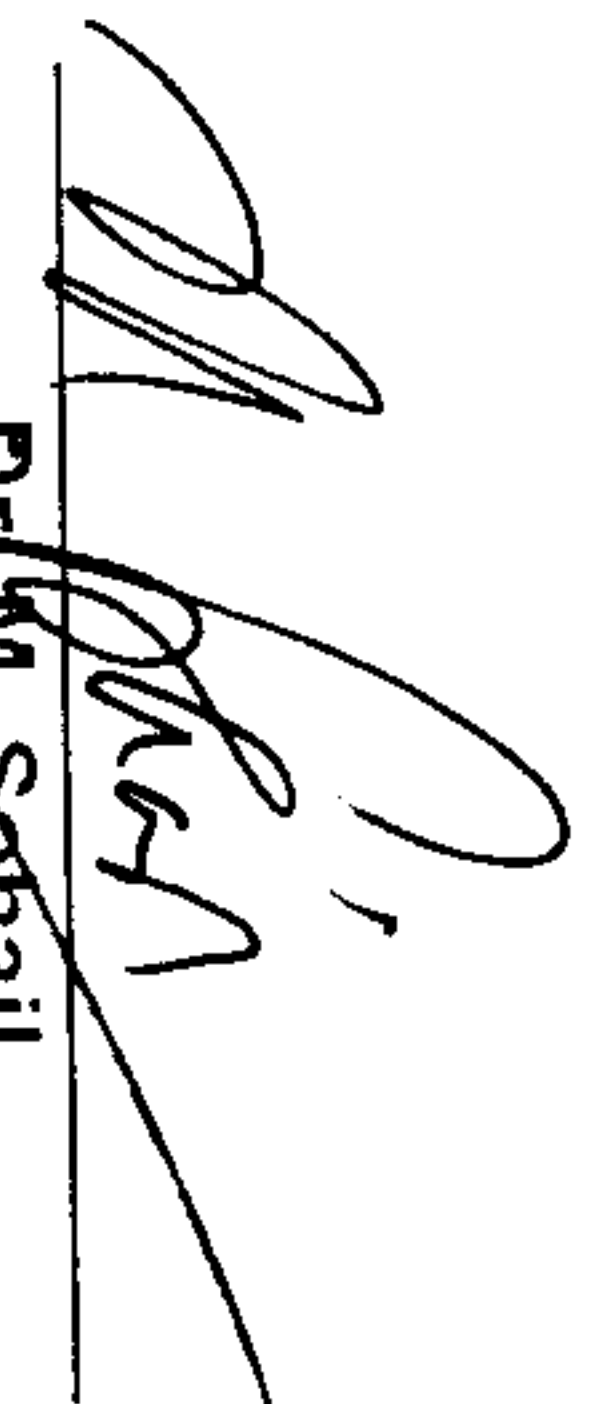
*[Handwritten signatures and initials]*

Technical Eligibility of Product:	Not Eligible	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Not Eligible
Technical Eligibility of Firm:	Eligible	Eligible	Eligible	Eligible	Eligible	Not Eligible	Not Eligible
BID STATUS:	Non Responsive	Responsive	Responsive	Responsive	Non Responsive	Non Responsive	Non Responsive

  
Mr. Haseeb Aslam  
 BioMedical Engineer  
 Nominated by SHC&ME Department, Lahore  
 (Member)

  
Electronic Equipment Care Taker  
 F.I.C. Faisalabad  
 (Member)

  
AMS (P&D)  
 F.I.C. Faisalabad  
 (Member)

  
Dr. M. Sohail  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

Head of Cardiology Department  
 F.I.C. Faisalabad  
 (Chairman)

**BID EVALUATION SHEET/TECHNICAL SHEET**

NAME OF THE EQUIPMENT: Cardiac Monitor (3B)

**PART-I  
KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron	IBM
1	Complete Package/Tender	Yes	Yes	Yes	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II

*(Handwritten signatures and initials)*

PART- II

Sr. No.	Evaluation Parameters	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron	IBM
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	Yes	Yes	Yes	Yes	No legal attested sole authorization	No legal attested sole authorization	No legal attested sole authorization
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes	Yes	No Technical trained engineers	No Technical trained engineers
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes		Yes	No	No
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	Yes	Yes	Yes	No Satisfactory Report Attached	No Satisfactory Report Attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes	Yes	No Warranty from the manufacturer	No Warranty from the manufacturer
	Remarks:	Eligible for part III	Not Eligible for part III	Eligible for part III	Eligible for part III	Not Eligible for part III	Not Eligible for part III	Not Eligible for part III

*[Handwritten signatures and initials]*

PART - III


SPECIFICATION COMPLIANCE /EVALUATION PARAMETERS


Name of Equipment	COMPANY	Total Technology	Friends Traders	Mediland Pakistan	Mediquips	Radiant	Varitron	IBM
Cardiac Monitor (3B)	Manufacturer	Edan Instrument	Mindray	Philips	Nihon Kohden	Biolight	Spacelab	Creative Medical
	Model	iM80	Umec 15	Effcia CM150	Lifescopce-TR (BSM-6701K)	Q7	Series Exprezzon	UP-9000
Country of Manufacturer		China	China	USA	Japan	China	USA	China
Country of Origin of Product/Model Number		China	China	Netherland	Japan	China	USA	China
Compliance with defined quality standards		Yes	Yes	Yes	Yes		No FDA 510K & CE	No FDA 510K
Specification Compliance features wise:								
Specifications:		Monitor launch date is Nov 2011 as mentioned on FDA 510K summary which is 8 years old instead of maximum 5 years	Yes	Yes	Yes	No Monitor is not intended for pediatric patients arrhythmia and ST Analysis as clearly mentioned on FDA 510K summary	No External battery backup (UPS) offered Attached FDA 510 K is for model 91393 whereas quoted model is different CE Declaration attached instead of CE Certificate from 3 <sup>rd</sup> party notifying body	No

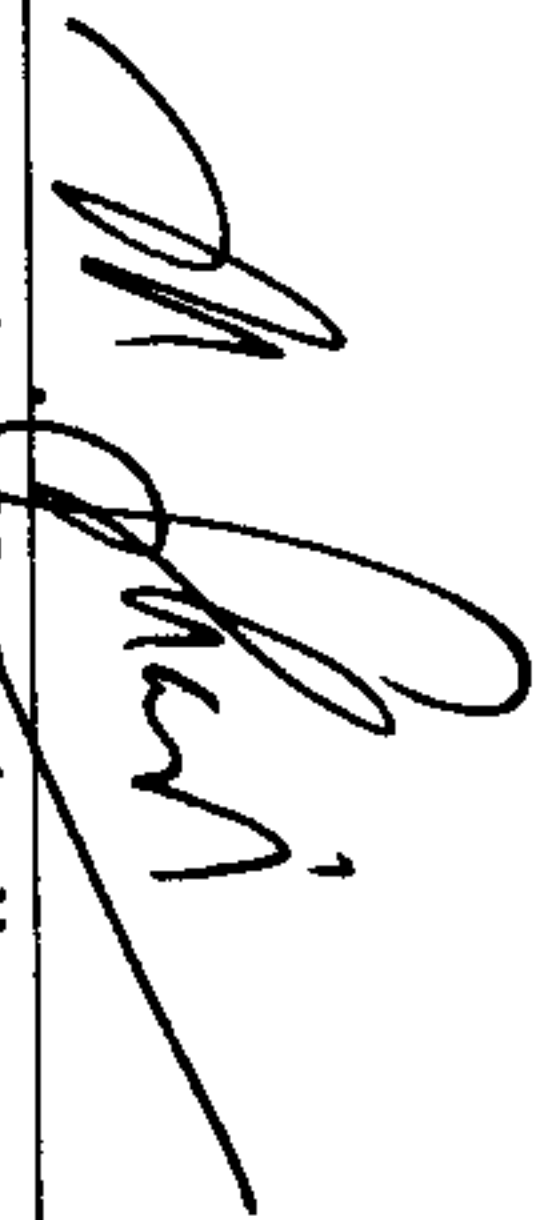
*[Handwritten signatures and initials]*




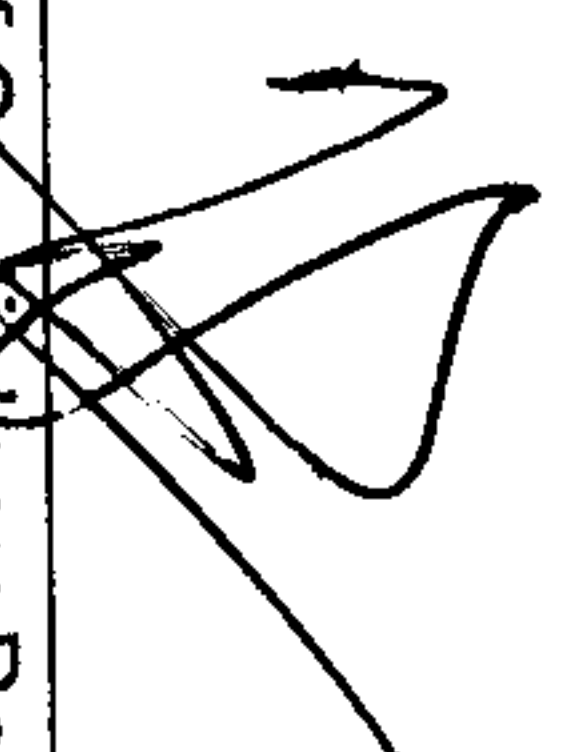
Technical Eligibility of Product:	Not Eligible	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Not Eligible
Technical Eligibility of Firm:	Eligible	Eligible	Eligible	Eligible	Not Eligible	Not Eligible	Not Eligible
<b>BID STATUS:</b>	<b>Non Responsive</b>	<b>Responsive</b>	<b>Responsive</b>	<b>Responsive</b>	<b>Non Responsive</b>	<b>Non Responsive</b>	<b>Non Responsive</b>

  
Mr. Haseeb Aslam  
 BioMedical Engineer  
 Nominated by SHC&ME Department, Lahore  
 (Member)

  
Electronic Equipment Care Taker  
 F.I.C. Faisalabad  
 (Member)

  
Dr. M. Sohail  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
AMS (P&D)  
 F.I.C. Faisalabad  
 (Member)

  
Head of Cardiology Department  
 F.I.C. Faisalabad  
 (Chairman)

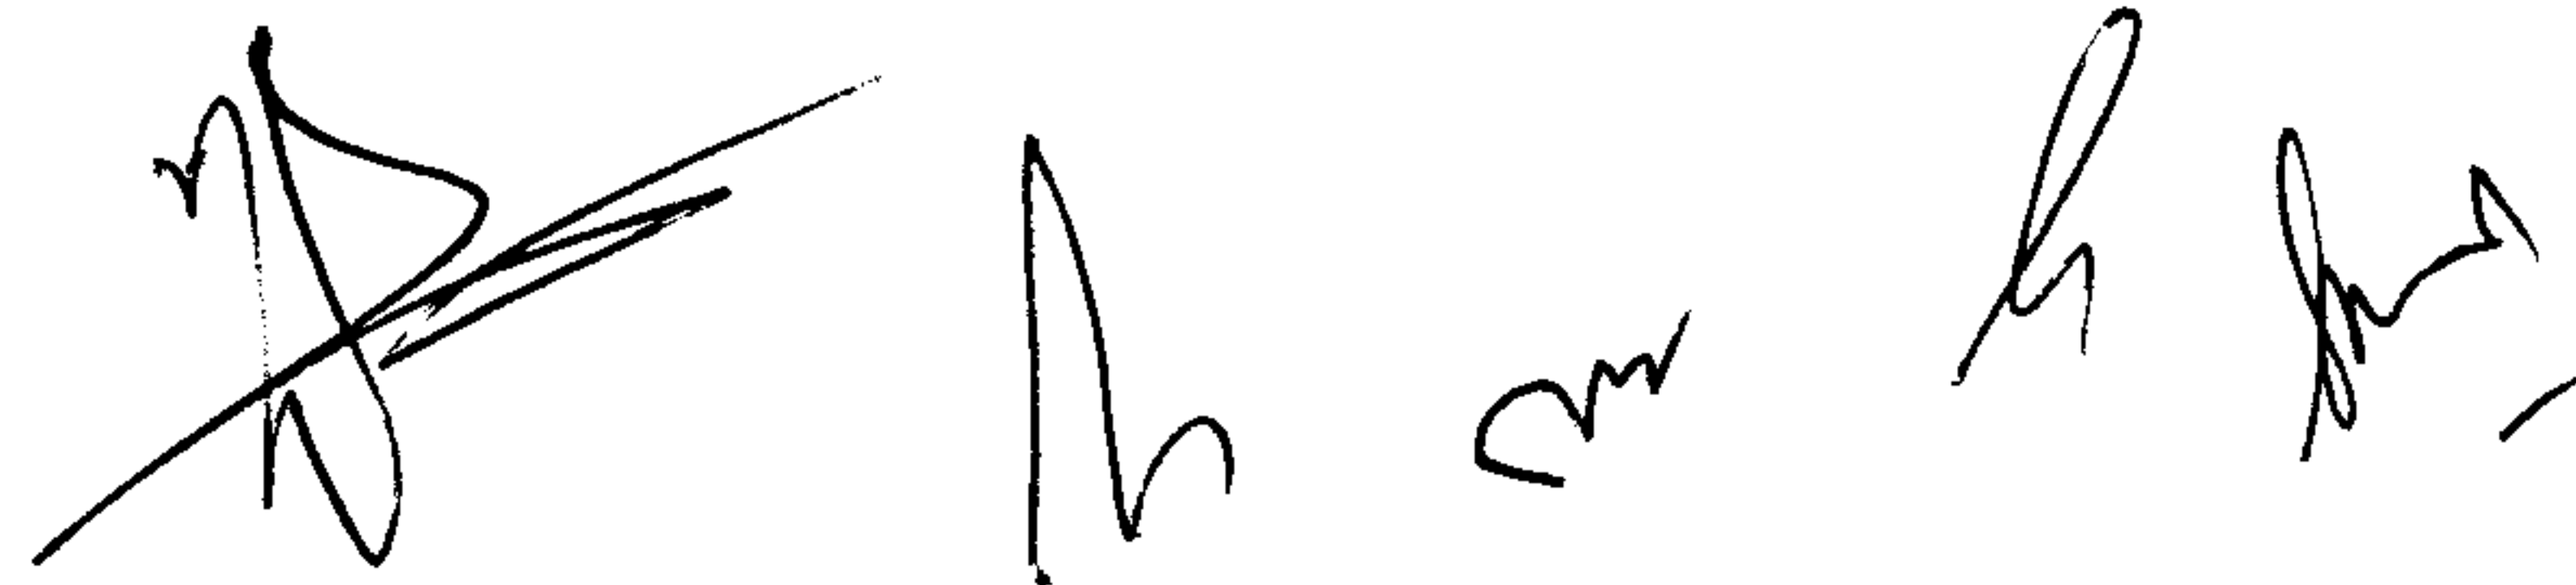
## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: INTRA AORTIC BALLOON PUMP

PART- I

KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)

Sr. No.	Evaluation Parameters	UDL	Mediland Pakistan
1	Complete Package/Tender	Yes	Yes
2	Original Receipt of Tender	Yes	Yes
3	Affidavit from Bidder	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes
6	Delivery Period	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II




**PART- II**


Sr. No.	Evaluation Parameters	UDL	Mediland Pakistan
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	No Embassy attested authorization	Yes
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	The firm was asked by BME and DMS (Purchase) to participate in Repair & Maintenance of Arrow Bran IABP but they refused	Yes
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes
6	Compliance of Warranty as per tender	No 5 year comprehensive warranty from manufacturer not offered	Yes
	Remarks:	Not Eligible for part III	Eligible for part III

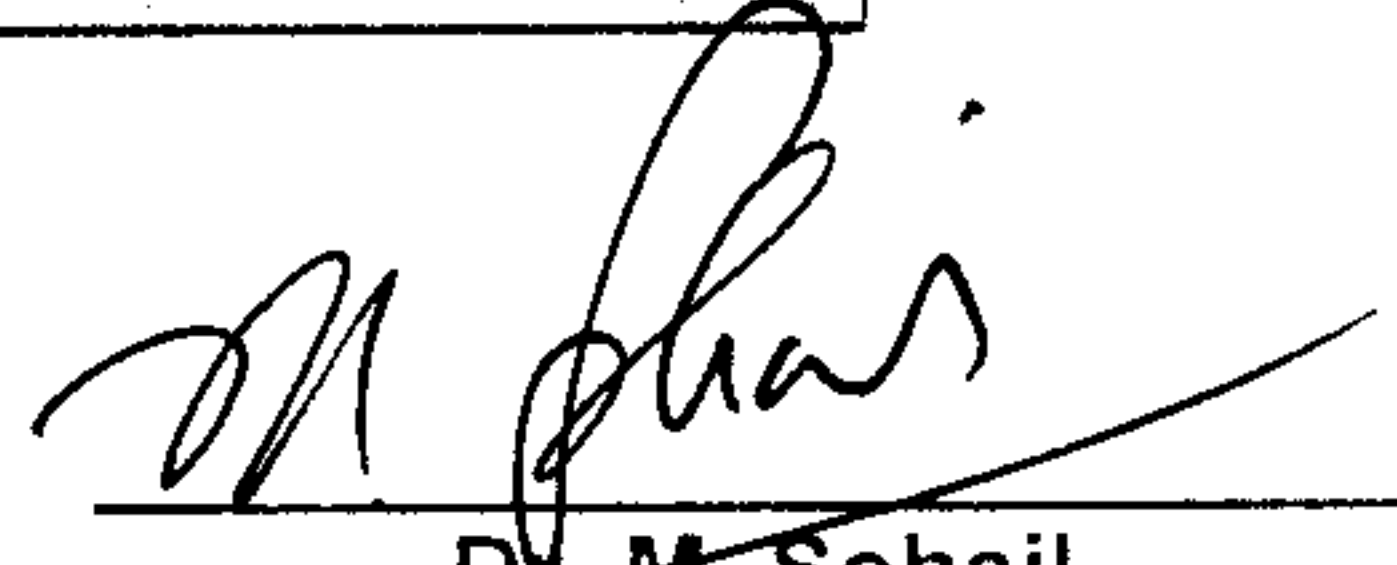
*[Handwritten signatures and initials]*

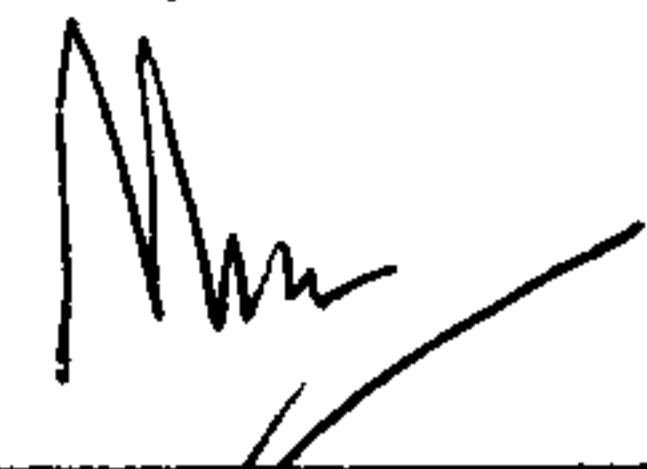
PART – III

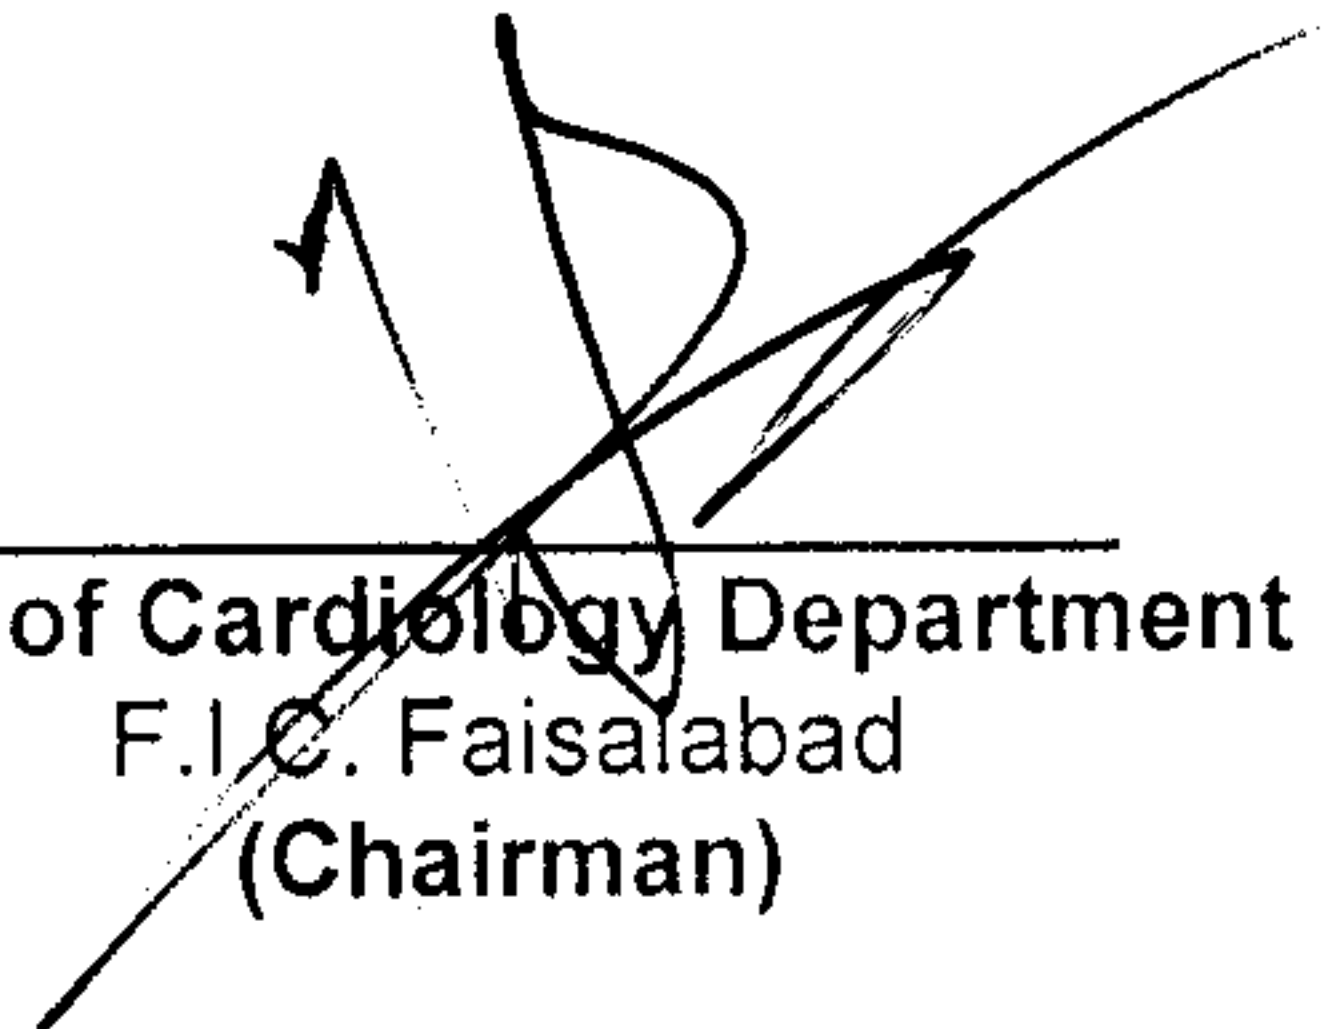
Name of Equipment	COMPANY	UDL	Mediland Pakistan
<u>Intra Aortic Balloon Pump</u>	Manufacturer	Arrow Int	Getinge Group Datascope
	Model	Arrow AC3 Optimus	Cardiosave hybrid
Country of Manufacturer		USA	Sweden
Country of Origin of Product/Model Number		USA	USA
Compliance with defined quality standards		Yes	Yes
Specification Compliance features wise:			
Specifications:		No control of deflation point in automatic mode	Yes
Technical Eligibility of Product:		Not Eligible	Eligible
Technical Eligibility of Firm:		Not Eligible	Eligible
BID STATUS:		Non Responsive	Responsive

  
**Mr. Haseeb Aslam**  
**BioMedical Engineer**  
 Nominated by SHC&ME Department,  
 Lahore  
 (Member)

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
 (Member)

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
 (Member)

  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
 (Chairman)

## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: HYPO/HYPER THERMIA MACHINE

**PART- I**

**KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)**

Sr. No.	Evaluation Parameters	Medica	Mediland Pakistan	Universal Enterprises
1	Complete Package/Tender	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II

*[Handwritten signatures and marks]*


PART- II


Sr. No.	Evaluation Parameters	Medica	Mediland Pakistan	Universal Enterprises
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	Yes	Yes	No Embassy Attested Authorization
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	No Certificate of technical trained engineers attached
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	No Sale reference/satisfactory report attached
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes
	Remarks:	Eligible for part III	Eligible for part III	Not Eligible for part III


*[Handwritten signatures and initials]*

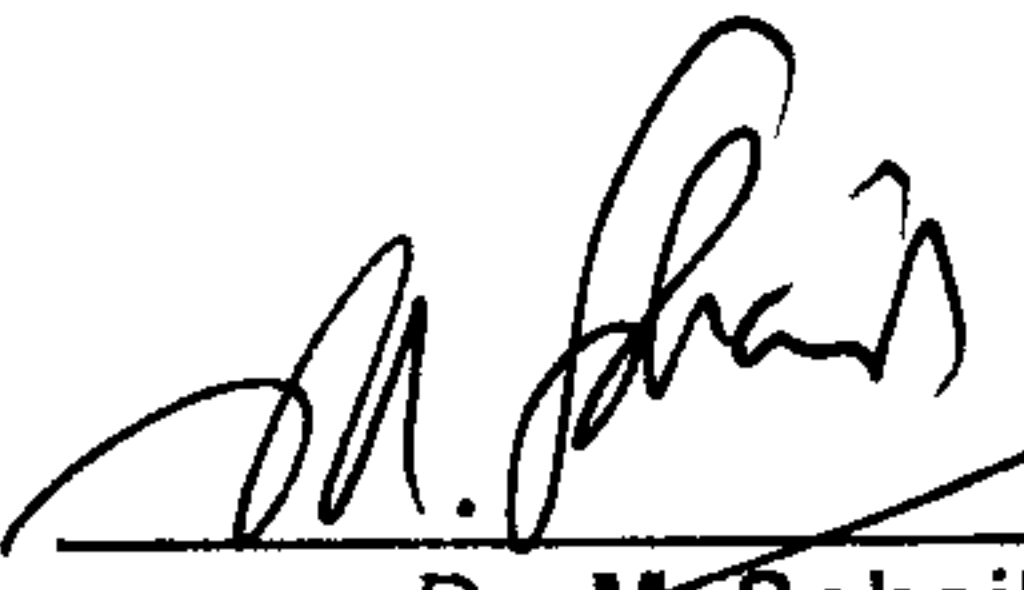
PART – III


Name of Equipment	COMPANY	Medica	Mediland Pakistan	Universal Enterprises
Hypo/Hyperthermia Machine	Manufacturer	Liva Nova	Getinge Group	Cincinnati subzero
	Model	3T	HCU 40	400CE
Country of Manufacturer		Germany	Sweden	USA
Country of Origin of Product/Model Number		Germany	Germany	USA
Compliance with defined quality standards		Yes	Yes	Yes
Specification Compliance features wise:				
Specifications:		Yes	Yes	No Optional Blankets not offered
Technical Eligibility of Product:		Eligible	Eligible	Not Eligible
Technical Eligibility of Firm:		Eligible	Eligible	Not Eligible
BID STATUS:		Responsive	Responsive	Not Responsive

  
**Mr. Haseeb Aslam**  
**BioMedical Engineer**  
 Nominated by SHC&ME Department,  
 Lahore  
 (Member)

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
 (Member)

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
 (Member)

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
 (Chairman)

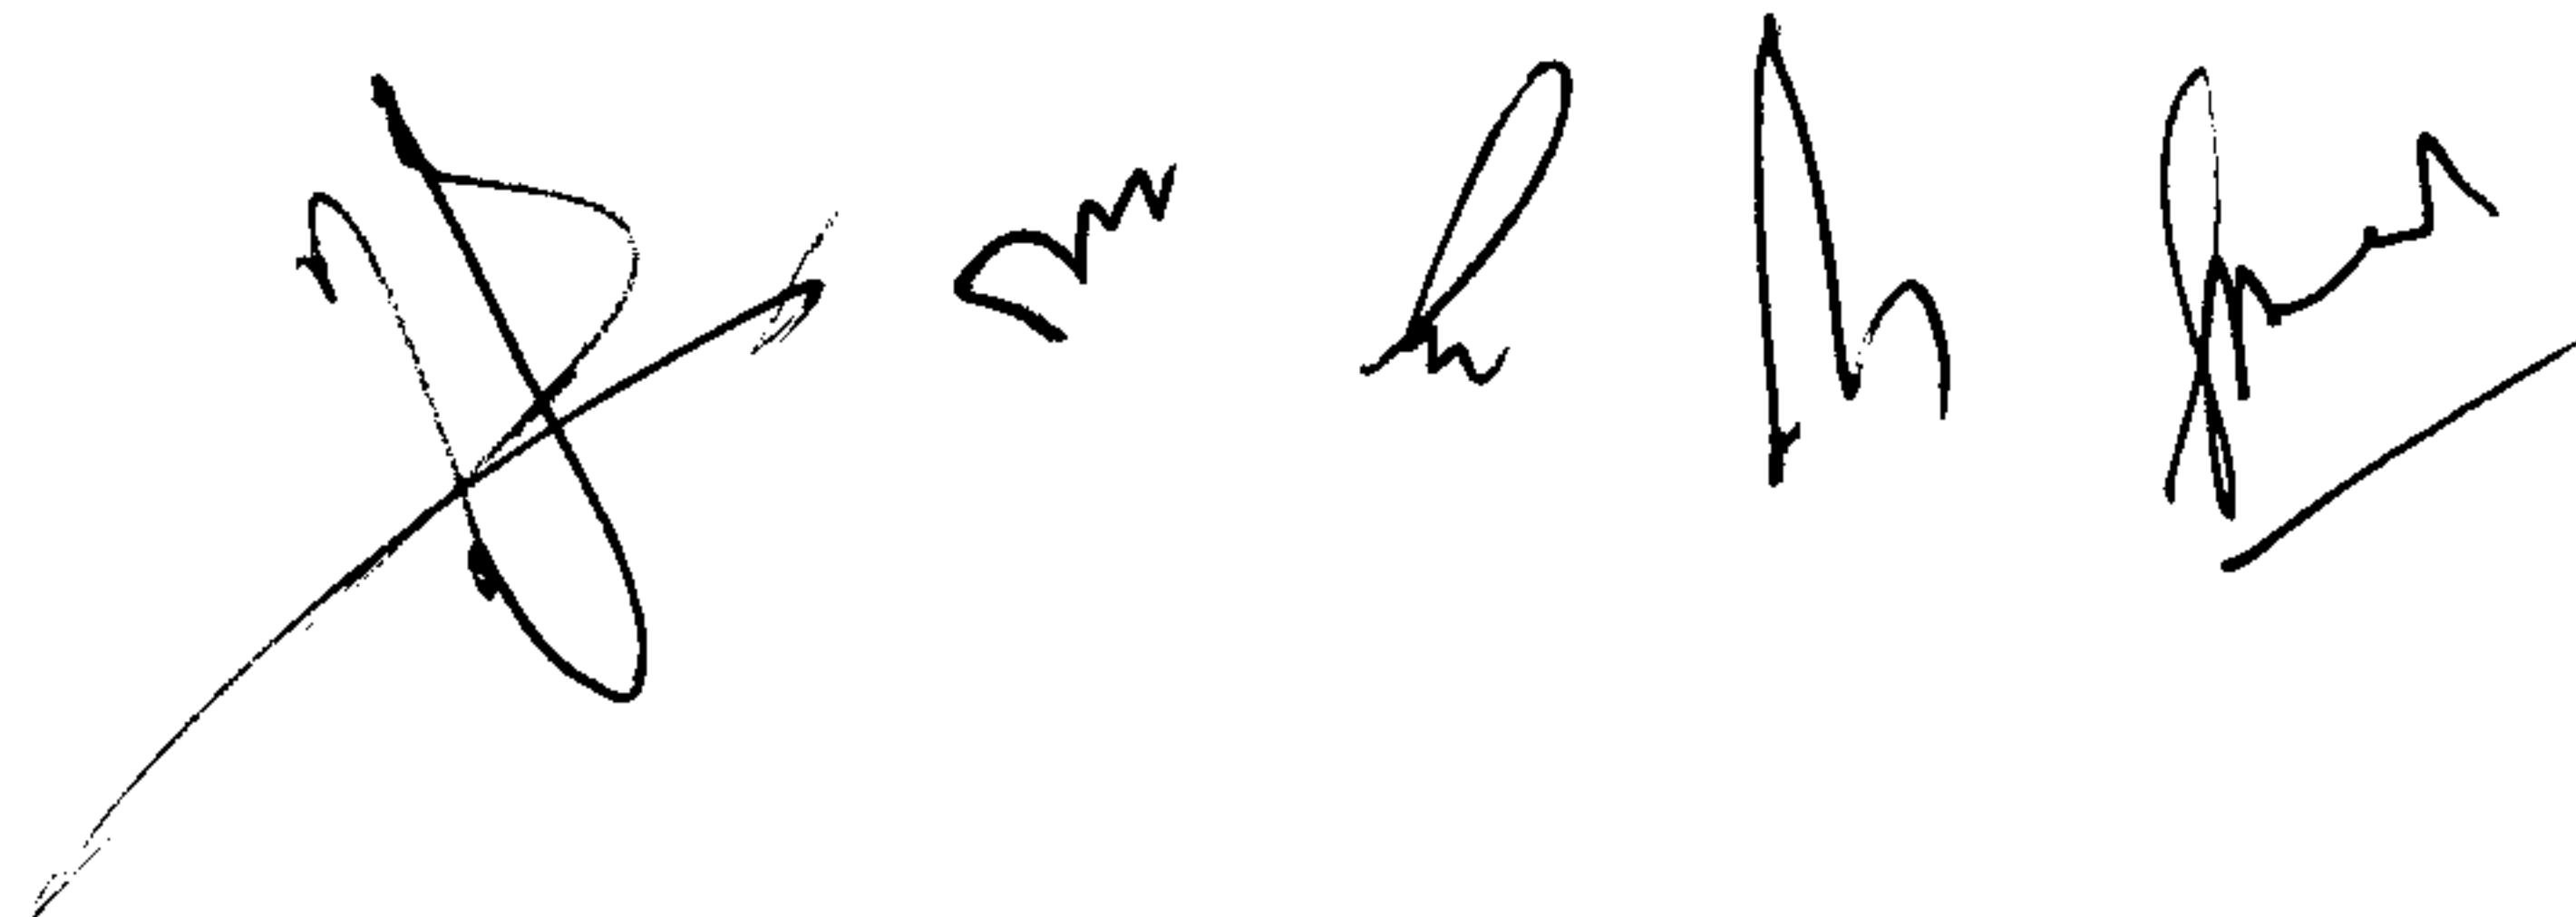
## BID EVALUATION SHEET/TECHNICAL SHEET

NAME OF THE EQUIPMENT: TEMPORARY PACE MAKER

### PART- I

#### KNOCK DOWN CRITERIA - (COMMERCIAL EVALUATION)

Sr. No.	Evaluation Parameters	Alliance Medical	Medtronic	Novatek Pakistan	Claris Medical
1	Complete Package/Tender	Yes	Yes	Yes	Yes
2	Original Receipt of Tender	Yes	Yes	Yes	Yes
3	Affidavit from Bidder	Yes	Yes	Yes	Yes
4	Bid Security	May be in Financial	May be in Financial	May be in Financial	May be in Financial
5	Bid Validity	Yes	Yes	Yes	Yes
6	Delivery Period	Yes	Yes	Yes	Yes
Remarks:		Eligible for part II	Eligible for part II	Eligible for part II	Eligible for part II

Handwritten signatures and initials in black ink, located at the bottom of the page. There are five distinct marks, including a large stylized signature on the left and several smaller initials or signatures to its right.



PART- II


Sr. No.	Evaluation Parameters	Alliance Medical	Medtronic	Novatek Pakistan	Claris Medical
1	Exclusive Authorization / Sole Agent Certificate by the Manufacturer	Yes	Yes	Yes	Yes
2	Technical & Engineering capability(As defined for the specific tender in specifications)	Yes	Yes	Yes	Yes
3	Certificate from the Manufacturer about the after sales services through agent or itself (In case specifically demanded in the specifications)	Yes	Yes	Yes	Yes
4	Vendor Past performance (In case of unsatisfactory performance, details must be mentioned)	Yes	Yes	Yes	Yes
5	Availability of relevant Tools and Testing / Calibration Equipment	Yes	Yes	Yes	Yes
6	Compliance of Warranty as per tender	Yes	Yes	Yes	Yes
	Remarks:	Eligible for part III	Eligible for part III	Eligible for part III	Eligible for part III

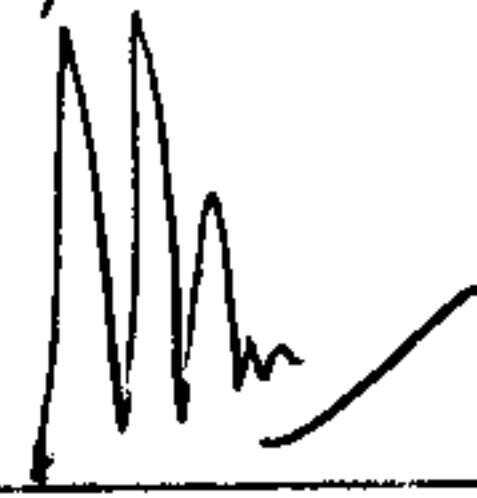
*h m h*


*[Handwritten signature]*

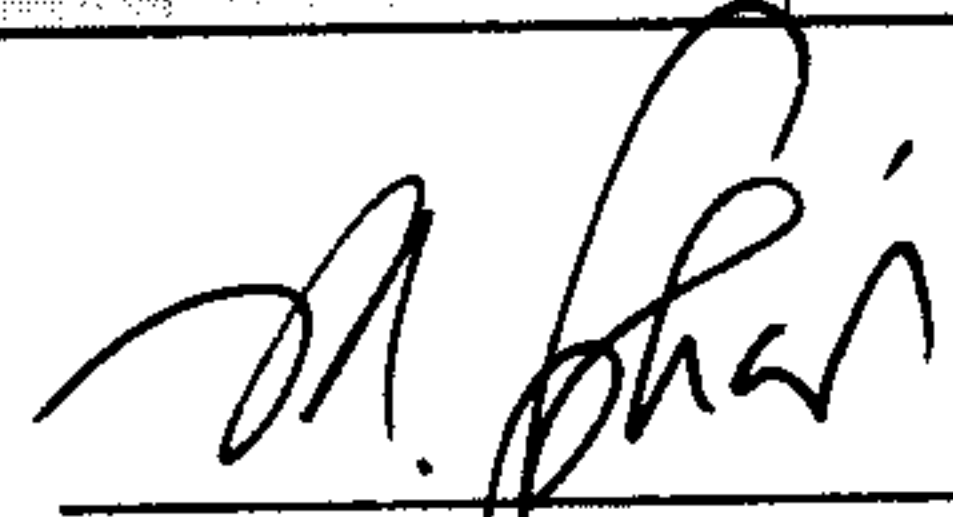
PART – III

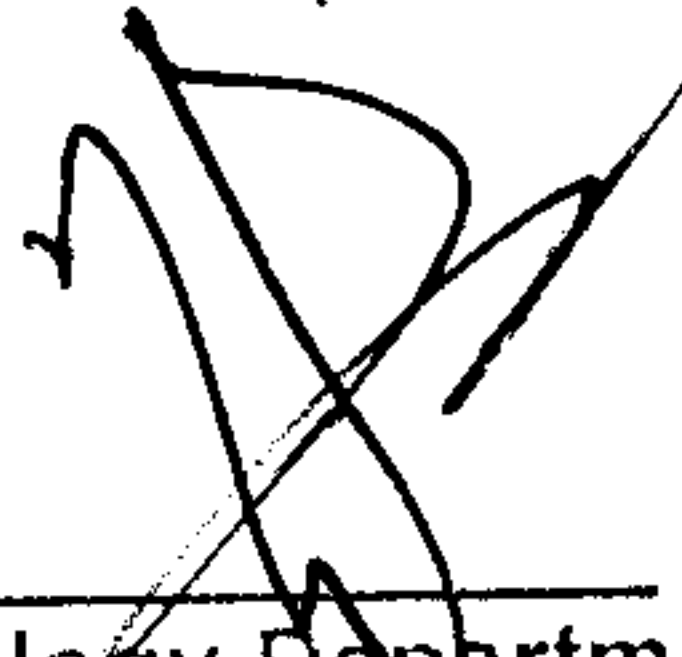
Name of Equipment	COMPANY	Alliance Medical	Medtronic	Novatek Pakistan	Claris Medical
TEMPORARY PACE MAKER	Manufacturer	Osypka AG	Medtronic	Livetec GmbH	Osypka Medical
	Model	Pace 101H	53401	T10	Pace 101
Country of Manufacturer		Germany	USA	Germany	Germany
Country of Origin of Product/Model Number		Germany	Malaysia	Germany	Germany
Compliance with defined quality standards		Yes	Yes	Yes	Yes
Specification Compliance features wise:					
Specifications:		No backup operation during battery change	No DRAP Registration	Yes	No DRAP Registration No backup operation during battery change
Technical Eligibility of Product:		Not Eligible	Not Eligible	Eligible	Not Eligible
Technical Eligibility of Firm:		Eligible	Eligible	Eligible	Eligible
BID STATUS:		Non Responsive	Non Responsive	Responsive	Non Responsive

  
**Mr. Haseeb Aslam**  
**BioMedical Engineer**  
 Nominated by SHC&ME Department,  
 Lahore  
 (Member)

  
**AMS (P&D)**  
 F.I.C. Faisalabad  
 (Member)

  
**Electronic Equipment Care Taker**  
 F.I.C. Faisalabad  
 (Member)

  
**Dr. M. Sohail**  
 Assistant Prof. Cardiac Surgery  
 F.I.C. Faisalabad  
 (Member)

  
**Head of Cardiology Department**  
 F.I.C. Faisalabad  
 (Chairman)