

**MINUTES OF THE MEETING REGARDING RE-EVALUATION OF CARDIAC SURGICAL DISPOSABLE ITEMS  
NO. 3,5,6,7,19,20,21,22,23,24,26,62,68,76,78,88,91,93,146 AND 147 HELD ON 11.11.2020 IN THE  
CONFERENCE ROOM, FIC, FAISALABAD FOR THE F.Y 2020-2021.**


Following members attended the meeting.

- 1 **Dr. Hamid Saeed**, Head of Cardiology, F.I.C. Faisalabad.
- 2 **Dr. Muhammad Sajid**, AMS (Purchase/Stores), F.I.C. Faisalabad.
- 3 **Dr. Husnain Zafar**, Assistant Professor of Cardiac Surgery, FIC, Faisalabad
- 4 **Dr. Zaigam Rasool**, Assistant Professor of Cardiac Surgery (Peads), FIC, Faisalabad.
- 5 **Dr. Asghar Ali**, Anesthetist, FIC, Faisalabad.
- 6 **Miss. Iqra Liaqat**, Pharmacist, F.I.C. Faisalabad.
- 7 **Mr. Najam Ul Hassan**, Electronic Equipment Care Taker, F.I.C. Faisalabad.

**Agenda:**

The meeting was called on the recommendation of Grievance committee for the re-evaluation of following products.

1. M/s Imtiaz Brothers				
Item #	Item Name	Brand Name	Manufactured By / Imported By	Remarks
78	OXYGEN MASK ALL SIZES	Max	Anhui Ganor Medical Device Co, Ltd. China	T.A
2. M/s Anax Associates				
21	CARDIO VASCULAR DRAPE SET	Medpro Cardio Vascular Drape Set	Medpro, China	T.N.A Poor quality
3.M/s Husnain Pharma				
3	ADHESIVE DRESSING ROLL 4" (10CM x 10M/9.14M)	Hospital & Homecare (10CMX10M)	China	T.N.A Poor Stickiness
19	CANNULA NASAL FOR OXYGEN DELIVERY -ADULT	Flexicare	Flexicare Medical UK	T.N.A 1.Punjab Govt. experience not attached 2. Could not maintain desired flow rate
76	NEBULIZER KITS ALL SIZES	Maxineb	Flexicare Medical Limited UK	T.N.A 1.Punjab Govt. experience not attached 2. Could not maintain desired flow rate

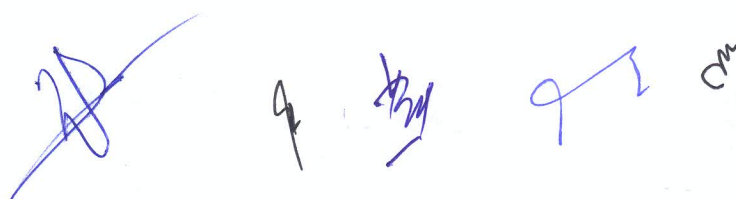

**4.M/s Ali Medical Store**

3	ADHESIVE DRESSING ROLL 4" (10CM x 10M/9.14M)	Fixomull Stretch (10CM x 10M)	Essity Pakistan Limited	<b>T.A</b>
---	---	----------------------------------	----------------------------	------------

**5. M/s Superior Healthcare International**

78	OXYGEN MASK ALL SIZES	Well Lead Medical/China	China	<b>T.N.A</b> In-sufficient Punjab Govt. experience attached
----	-----------------------	----------------------------	-------	---

**6.M/s Flowtronix System**

5	ANTI GRADE CARDIOPLEGIA CANNULA FOR PEADS (18G, 16G, 14G) without vent line	Andocor	Belgium	<b>T.N.A</b> 1.Stylet does not rotate appropriate during procedure 2.Punjab Govt. experience not attached
6	ANTI GRADE CARDIOPLEGIA CANNULA WITH VENT LINE ADULT	Andocor	Belgium	<b>T.N.A</b> 1.Stylet does not rotate appropriate during procedure
7	AORTIC CANNULA ANGLED TIP WIRE REINFORCED ALL SIZES (PEADS) APPROVED BY FDA / CE	Andocor	Belgium	<b>T.N.A</b> Metal tip not required
20	CARDIOPLEGIA DELIEVERY SYSTEM 1:4 & 1:8 Ratio (According to FIC Diagram)	Nipro		<b>T.N.A</b> 1.In technical offer country of origin not mentioned 2.Not according to FIC drawing and ¼ line not attached in the circuit
21	CARDIO VASCULAR DRAPE SET	Allmed	Hefei C & P nonwoven	<b>T.N.A</b> Poor quality
22	CENTRAL VENOUS CATHERIZATION SET TRIPLE LUMEN 7FR	Able/Guangdone Baihe Medical	China	<b>T.N.A</b> The line is too soft liable to kink
23	CENTRAL VENOUS CATHERIZATION SET SINGLE LUMEN 7FR	Able/Guangdone Baihe Medical	China	<b>T.N.A</b> The line is too soft liable to kink
24	CENTRAL VENOUS CATHERIZATION SET TRIPLE LUMEN 5.5FR	Able/Guangdone Baihe Medical	China	<b>T.N.A</b> The line is too soft liable to kink
26	CHEST DRAINAGE BOTTLE (3- Chamber for open heart surgery)	Alleva Medical	Hongkong	<b>T.N.A</b> 1. Punjab Govt. experience not attached 2. Medical device registration not attached 3. Hard silicon tubing
62	HEMODIALYSIS CATHETER DOUBLE LUMEN	Able/Guangdon Baihe Medical	China	Medical device registration of Hemodialyzer attached not for Double Lumen Catheter
68	ISOLATOR WITH LOOP	Tpri		<b>T.N.A</b> 1. M/s Flowtronix does not have authority letter for this product as M/s Imtiaz Brothers

				also quoted same brand and they have authority for this product from manufacturer
88	PRESSURE TRANSDUCER FOR HEART LUNG MACHINE COMPATIBLE WITH TERUMO MACHINE OR EQUIVALENT	Able Guangdong Baihe Medical	China	<b>T.N.A</b> Not compatible with machine
91	PTFE PATCH (0.1mm)	Bard	USA	<b>T.A</b>
93	REINFORCED SURGEON GOWN (FRONT & ARMS) ALL SIZES DISPOSABLE	Allmed	Hefei C & P nonwoven	<b>T.N.A</b> 1.In-sufficient Punjab Govt. experience attached 2.Poor quality
146	PRESSURE TRANSDUCER KIT WITH STAND AND LEAD	Guangdong Baihe Medical	China	<b>T.N.A</b> Not compatible with machine
147	CARDIAC SUMP FOR PEADS WITH CONNECTER	Andocor	Belgium	<b>T.N.A</b> 1.Metal tip not required for peads and diameter too large 2.Punjab Govt. experience not attached



Mr. Najam Ul Hassan ,  
Electronic Equipment Care Taker  
F.I.C. Faisalabad.




Miss. Iqra Liaqat,  
Pharmacist,  
F.I.C. Faisalabad.

Dr. Asghar Ali,  
Anesthetist  
F.I.C. Faisalabad.


Dr. Zaigam Rasool ,  
Assistant Professor of  
Cardiac Surgery (Peads),  
FIC, Faisalabad.



Dr. Husnain Zafar,  
Assistant Professor of Cardiac  
Surgery,  
FIC, Faisalabad



Dr. Muhammad Sajid,  
AMS (Purchase/Stores),  
FIC, Faisalabad



Dr. Hamid Saeed,  
Head of Cardiology  
F.I.C. Faisalabad.