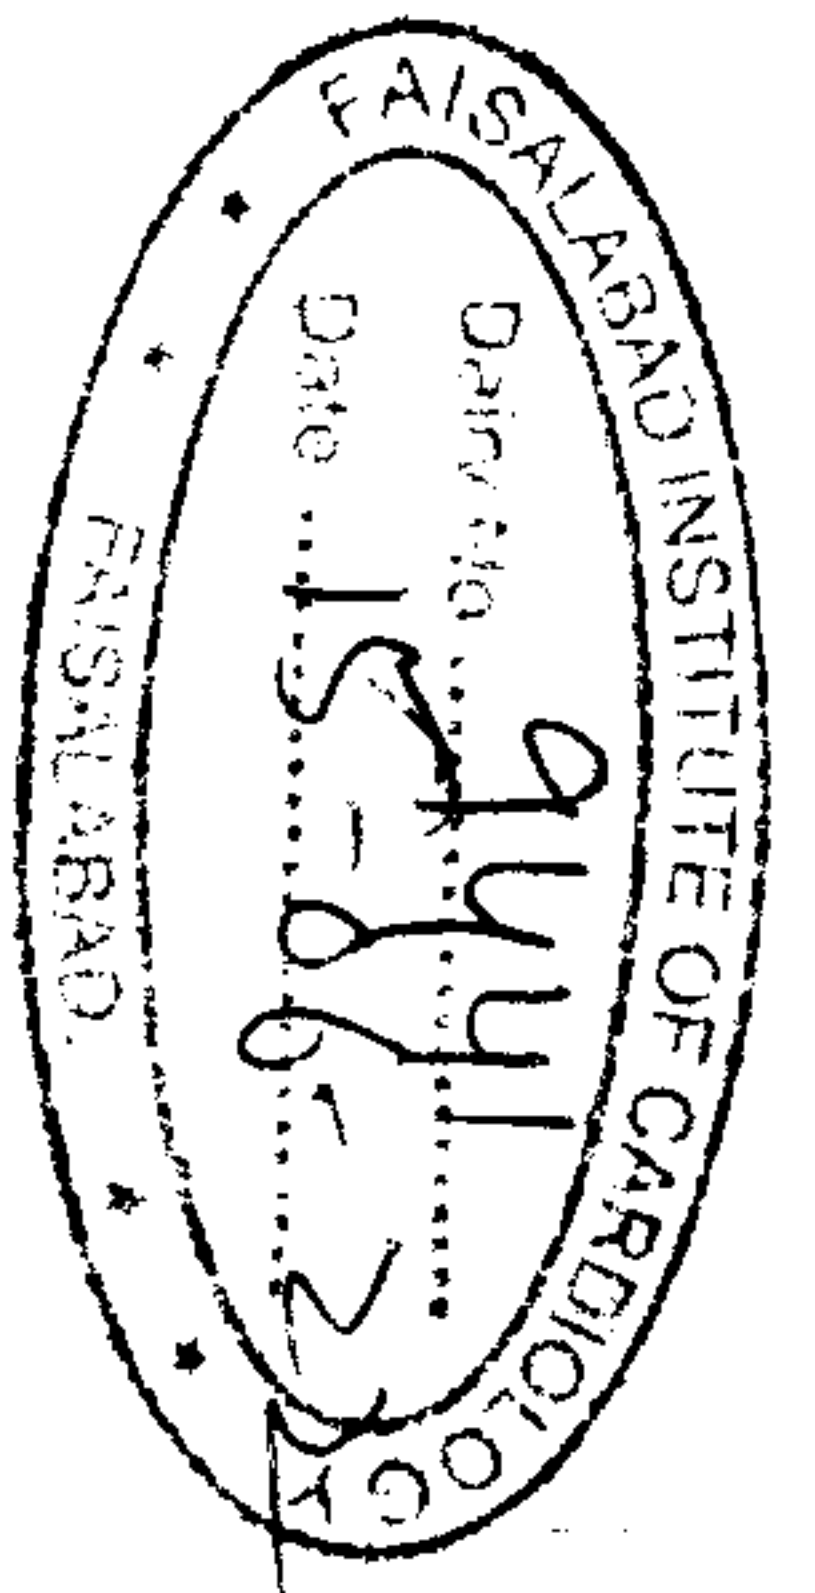


**MINUTES OF GRIEVANCE COMMITTEE MEETING  
FAISALABAD INSTITUTE OF CARDIOLOGY, FAISALABAD**



A meeting of Grievance Committee for product of Angiography/Angioplasty Items F.Y. 2022-23 was held on 08-06-2022 at 10:00AM in the Office of the Medical Superintendent, Faisalabad Institute of Cardiology, Faisalabad.

**ANGIOGRAPHY/ANGIOPLASTY**

**M/s Alliance Medical**

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
4	CLOT ASPIRATION CATHETER	Extractor	Genoss Ltd. Korea	Authority letter from manufacturer not notarized attached	Authority letter from manufacturer notarized attached	Accepted
15	GUIDE WIRE 150-160 CM STANDARD LENGTH 0.035 J TIP	Shunmei Medical	China	1. Authority letter from manufacturer not notarized attached 2. Free sale certificate not Embassy attested attached 3. Product list not attached in EC certificate 4. Stiff material	1. Authority letter from manufacturer notarized attached 2. Free sale certificate Embassy attested attached 3. Product list attached in EC certificate 4. End user Reservation	Rejected
16	GUIDE WIRE EXCHANGE LENGTH 0.035 260CM J TIP	Shunmei Medical	China	1. Authority letter from manufacturer not notarized attached 2. Free sale certificate not Embassy attested attached 3. Product list not attached in EC certificate 4. Stiff material	1. Authority letter from manufacturer notarized attached 2. Free sale certificate Embassy attested attached 3. Product list attached in EC certificate 4. End user Reservation	Rejected
19	INFLATION DEVICE WITH (Y-CONNECTOR) (INTRODUCER)	Genoss	Korea	Authority letter from manufacturer not notarized attached	Authority letter from manufacturer notarized attached	Accepted

Handwritten signatures and initials at the bottom of the page, including 'PC', 'J', and several illegible signatures.

NEEDLE)  
(TORQUER)  
40 TEMPORARY  
PACEMAKER LEAD

Dispomedica Germany

1. Authority letter from manufacturer not notarized attached

2. On technical offer manufacturer name Dispomedica while on DRAP registration, another manufacturer name mentioned

3. No experience with this institute (as supply pending)

1. Authority letter from manufacturer notarized attached

2. The MDR with the name Dispomedica as mentioned on technical offer provided

Rejected

41 TRANSFEMORAL SHEATH (SHEATH CATHETER WITH HAEMOSTATIC VALVE, GUIDE WIRE SPRING TYPE (J TYPE), DILATOR KINK RESISTANT, SELDINGER NEEDLE 18G WITH VALVE, IV CATHETER AND SCALPEL) ALL SIZES CE Approved Only

Shunmei Medical China

1. Authority letter from manufacturer not notarized attached

2. Product list not attached in EC certificate

3. Free sale certificate not Embassy attested attached

4. Valve leakage

3. No experience with this institute (End user Reservation)

1. Authority letter from manufacturer notarized attached

2. Product list attached in EC certificate

3. Free sale certificate Embassy attested attached

4. End user reservation

Rejected

42 TRANSRADIAL SHEATH (SHEATH CATHETER WITH HAEMOSTATIC VALVE, GUIDE WIRE (ST. TYPE), DILATOR KINK RESISTANT, SELDINGER NEEDLE 21G WITH VALVE, IV CATHETER AND SCALPEL)- ALL SIZES CE Approved Only

Shunmei Medical China

1. Authority letter from manufacturer not notarized attached

2. Product list not attached in EC certificate

3. Free sale certificate not Embassy attested attached

4. Valve leakage

1. Authority letter from manufacturer notarized attached

2. Product list attached in EC certificate

3. Free sale certificate Embassy attested attached

4. End user reservation

Rejected

3: PULMONARY VAOS II Osypka AG, Authority letter from Manufacturer not notarized attached  
 VALVULOPLASTY Germany  
 BALLOONS ALL  
 SIZES (SOFT  
 PROFILE) notarized attached  
 Accepted

M/s ATCO Pharma International (Pvt) Ltd.

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
31	PTCA BALLOON MONORAIL (SEMI COMPLIANT) - ALL SIZES	Flydo	ALVIMEDICA TURKEY	On technical offer manufacturer name Alvimedica Turkey while on DRAP registration CID Itlay mentioned	MDR with complete name and address of manufacturer provided	Accepted

M/s Cardiac Care

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
29	PRESSURE TUBING FOR HEMO DYNAMIC MONITORING	PRO LONG TUBE	PRO Active, Itlay	Free sale certificate not attached	Invalid Free sale certificate attached	Rejected
54	ECG CHEST ELECTRODE FOR ETT	FIAB	Itlay	1. Poor Conduction 2. Invalid Free sale certificate attached	1. End User Reservation 2. Invalid Free sale certificate attached	Rejected
55	ECG CHEST ELECTRODE FOR MONITORING - ADULT	FIAB	Itlay	1. Poor Conduction 2. Invalid Free sale certificate attached	1. End User Reservation 2. Invalid Free sale certificate attached	Rejected

M/s Digital Imaging Systems

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
73	PDA DEVICES ALL SIZES	PDA Amplazer Device	Abbott Vascular, USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted
74	DELIVERY SYSTEM FOR PDA DEVICES ALL	Amplazer Delivery System for PDA	Abbott Vascular, USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted

*(Handwritten signatures and initials)*

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
75	ASD DEVICES (SEPTAL OCCLUDER) ALL SIZES	Amplatzer ASD Devices	Abbott Vascular USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted
76	DELIVERY SYSTEM FOR SEPTAL OCCLUDER DEVICES ALL SIZES	Amplatzer Delivery System for ASD	Abbott Vascular USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted
82	VSD DELIVERY SYSTEM ALL SIZES	Amplatzer Delivery System for VSD	Abbott Vascular USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted
83	VSD DEVICES ALL SIZES	Amplatzer VSD Devices	Abbott Vascular USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted
89	ASD SIZING BALLOON (24 FR, 34 FR)	Amplatzer Sizing Balloon	Abbott Vascular USA/Europe	Invalid FDA certificate attached	Valid FDA certificate attached	Accepted

**M/s Ferozsons Laboratories Ltd**

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
10	DIAGNOSTIC CATHETER (5FR AND 6FR) & ALL TYPES	Impulse	Boston Scientific, USA	1. Not sufficient sample provided for evaluation 2. Medical device registration not attached 3. Invalid Free sale certificate attached	1. Not sufficient sample provided for evaluation 2. Medical device registration not attached 3. Invalid Free sale certificate attached	Rejected
11	DISTAL PROTECTION DEVICE (FILTERTYPE) ALL SIZES	EZ	Boston Scientific, USA	1. FDA certificate not attached 4. No experience with this institute	Invalid Free sale certificate attached	Rejected
12	DRUG ELUTING BALLOON ALL SIZES (FDA APPROVED)	Agent (CE Mark)	Boston Scientific, USA	1. FDA certificate not attached 2. Medical device registration not attached	1. FDA certificate not attached 2. Medical device registration not attached	Rejected

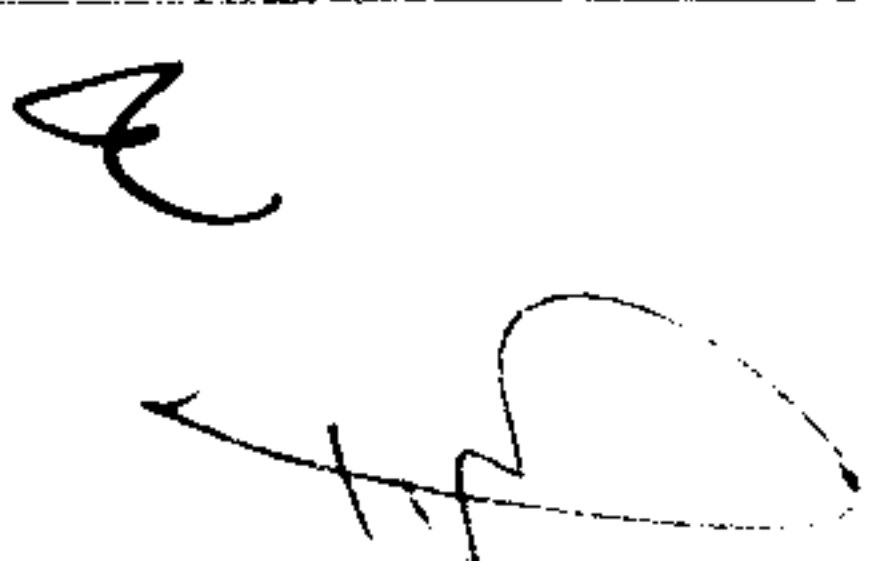



*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*

*[Handwritten signature]*

49	INFLATION DEVICE WITH (Y-CONNECTOR) (INTRODUCER NEEDLE) (TORQUER)	Advantage Encore 26	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. registration not attached</li> <li>2. Free sale certificate not attached</li> <li>3. Not user friendly</li> <li>4. EC certificate not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Invalid Free sale certificate attached (23-03-2022)</li> <li>2. End User Reservation</li> <li>3. EC attached</li> </ul>	Rejected
25	PERIPHERAL BALLOON (MONORAIL) - ALL SIZES	Mustang	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. Free sale certificate not attached</li> <li>3. EC certificate not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. Free sale certificate not attached</li> <li>3. EC certificate attached</li> </ul>	Rejected
26	PERIPHERAL STENTS (SELF EXPANDABLE/ BALLOON EXPANADABLE) - ALL SIZES	Express	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. Free sale certificate not attached</li> <li>3. EC certificate not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. Free sale certificate not attached</li> <li>3. EC certificate attached</li> </ul>	Rejected
30	PTCA BALLOON MONORAIL NON-COMPLIANT-ALL SIZES	NC Quantum Apex	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> </ul>	Rejected
31	PTCA BALLOON MONORAIL (SEMI COMPLIANT) - ALL SIZES	Maverick 2	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> </ul>	Rejected
32	PTCA BALLOON (OTW) SEMI COMPLIANT ALL SIZES	Emerge	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. EC certificate not attached</li> </ul>	<ul style="list-style-type: none"> <li>1. Medical device registration not attached</li> <li>2. EC certificate attached</li> </ul>	Rejected
33	PTCA GUIDE WIRE, HYDROPHILIC, NON TAPERED STANDARD STRAIGHT TIP, MODERATE SUPPORT, POLYMER	PT2 MS	Boston Scientific, USA	<ul style="list-style-type: none"> <li>1. Sample not provided</li> <li>2. No experience with this institute</li> </ul>	<ul style="list-style-type: none"> <li>1. Sample not provided</li> <li>2. End user Reservation</li> </ul>	Rejected

<p>COATED 0.014 AND 175-195 CM</p> <p>34 PTCA GUIDE WIRE WORK HORSE WIRE SOFT TIP, MODERATE SUPPORT, 0.014 AND 175-195 CM</p>	<p>PT Graphix 182cm</p> <p>Boston Scientific, USA</p>	<p>Not suitable as workhorse wire (HydroPhilic)</p>	<p>End user Reservation</p>	<p>Rejected</p>
<p>35 PTCA GUIDE WIRE WORK HORSE WIRE SOFT TIP, MODERATE SUPPORT, 0.014 AND 300 CM</p>	<p>PT Graphix 300cm</p> <p>Boston Scientific, USA</p>	<p>Not suitable as workhorse wire (HydroPhilic)</p>	<p>End user Reservation</p>	<p>Rejected</p>
<p>36 PTCA GUIDE WIRE, HYDROPHILIC, TAPERED, INTERMEDIATE STRAIGHT TIP, MODERATE SUPPORT, POLYMER COATED, 0.014 AND 175-195 CM</p>	<p>Hornet</p> <p>Boston Scientific, USA</p>	<p>1. Sample not provided 2. No experience with this institute 3. Medical device registration not attached 4. EC certificate not attached</p>	<p>1. Sample not provided 2. End user Reservation 3. MDR not attached 4. EC attached</p>	<p>Rejected</p>
<p>37 PTCA GUIDE WIRE, EXTRA SUPPORT WIRE, 0.014 AND 175-195 CM</p>	<p>Choice Extra Support</p> <p>Boston Scientific, USA</p>	<p>1. Sample not provided 2. No experience with this institute 3. Medical device registration not attached 4. EC certificate not attached</p>	<p>1. Sample not provided 2. End user Reservation 3. MDR not attached 4. EC attached</p>	<p>Rejected</p>
<p>38 CTO PCI GUIDE WIRES RADIO OPAQUE PART 15CM HYDROPHILIC COATING 40CM (I) TIP LOAD 1.5-2 GM</p>	<p>Fighter (Tip Load 1.5G)</p> <p>Boston Scientific, USA</p>	<p>1. Sample not provided 2. No experience with this institute 3. Medical device registration not attached 4. EC certificate not attached</p>	<p>1. Sample not provided 2. End user Reservation 3. MDR not attached 4. EC attached</p>	<p>Rejected</p>
<p>38 II. TIP LOAD 3-4.5</p>	<p>PT Graphix</p> <p>Boston</p>	<p>1. Sample not provided</p>	<p>3. Sample not provided</p>	<p>Rejected</p>

*[Handwritten signatures and initials at the bottom of the page]*

GM  
Supplier Support  
(Tip Load 3.6G) Scientific,  
USA

- 2. No experience with this institute
- 2. End user Reservation

- 3. Medical device registration not attached
- 3. MDR not attached

- 4. EC certificate not attached
- 4. EC attached

38 III. TIP LOAD - 4.5 GM  
PT  
GraphixStandard  
(Tip Load 5.3 G) Boston  
Scientific,  
USA

- 1. Sample not provided
- 1. Sample not provided
- 2. No experience with this institute
- 2. End user Reservation
- 3. Medical device registration not attached
- 3. MDR not attached

- 4. EC certificate not attached
- 4. EC attached

- 4. EC certificate not attached
- 4. EC attached

79 Glide Wire 0.035  
(Ordinary) Straight /  
curved Hydrophilic  
150CM Boston  
Scientific,  
USA

- 1. Free sale certificate not attached
- 1. Invalid Free sale certificate attached
- 2. Medical device registration not attached
- 2. Medical device registration not attached
- 3. No experience with this institute
- 3. End User reservation
- 4. Sample not provided
- 4. Sample not provided

- 3. No experience with this institute
- 3. End User reservation

80 Glide Wire  
Exchange Length  
0.035 & 0.025  
260CM Hydrophilic  
(Straight / Curved) Boston  
Scientific,  
USA

- 1. Free sale certificate not attached
- 1. Invalid Free sale certificate attached
- 2. Medical device registration not attached
- 2. Medical device registration not attached
- 3. No experience with this institute
- 3. End User reservation
- 4. Sample not provided
- 4. Sample not provided

- 3. No experience with this institute
- 3. End User reservation

81 Guide Wire Extra  
Stiff Exchange  
Length 0.035  
260CM (Super Stiff) Amplataz Super  
Stiff Wire Boston  
Scientific,  
USA

- 4. Sample not provided
- 4. Sample not provided
- EC certificate not attached
- EC certificate attached

88 FMBOIIZATION Vortex Coil Boston

- 1. Free sale certificate not attached
- 1. Invalid Free sale certificate

Accepted

*[Handwritten signatures and initials]*

COOLS ALL SIZES

Scientific  
USA

attached

attached

2. EC certificate not attached

2. EC certificate attached

M/s Friends Enterprises

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
54	ECG CHEST ELECTRODE FOR ETT	TOPTRACE	Ceracarta, Itlay	1. Invalid Free sale certificate attached 2. Poor quality	1. Invalid Free sale certificate attached 2. End user Reservation	Rejected
55	ECG CHEST ELECTRODE FOR MONITORING - ADULT	TOPTRACE	Ceracarta, Itlay	1. Invalid Free sale certificate attached 2. Poor quality	1. Invalid Free sale certificate attached 2. End user Reservation	Rejected
60	ECG Z FOLDER 100MM X 150MM	CARDIOLINE	United, Pakistan	1. License to manufacturer not attached 2. Free sale certificate not attached	1. License to manufacturer not attached 2. Free sale certificate not attached 3. Medical device registration is not compulsory parameter as this product fall in category of Medical device rules schedule A	Rejected
61	ECG Z FOLDER 110MM X 140MM	CERACARTA	Ceracarta, Itlay	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
64	STRIPS FOR GLUCOMETER (300 FOC GLUCOMETER REQUIRED COMPULSARY)	CareSens	I-Sens, Korea	Invalid Free sale certificate attached	Valid Free sale certificate attached	Accepted



M/s Health Tec  
Bid

Sr  
Company Name  
Bid Reject of M/s Health Tec

1 AC Observations  
1. Invalid DSL attached

GC Observation  
1. Renewal slip for DSL attached

Remarks  
Accepted

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
12	DRUG ELUTING BALLOON ALL SIZES (FDA APPROVED)	Protege	Blue Medical, Netherland	1. Authority letter from manufacturer not notarized attached 2. Medical device registration not attached	1. Authority letter from manufacturer notarized attached 2. Medical device registration not attached	Rejected

15	GUIDE WIRE 150-160 CM STANDARD LENGTH 0.035 J TIP	Acccoat 150cm	SP Medical, Denmark	1. Authority letter from manufacturer not notarized attached 5. Sample not provided	1. Authority letter from manufacturer notarized attached 5. Sample not provided	Accepted
----	---	---------------	---------------------	--	--	----------

16	GUIDE WIRE EXCHANGE LENGTH 0.035 260CM J TIP	Acccoat 260cm	SP Medical, Denmark	Authority letter from manufacturer not notarized attached	Authority letter from manufacturer notarized attached	Accepted
----	--	---------------	---------------------	---	---	----------

18	GUIDING CATHETER ALL SIZES & ALL TYPES	Primum; Hydrophilic Coated	Pendracare, Netherland	1. Medical device registration not attached 2. EC certificate not attached 3. Free sale certificate not attached	1. Medical device registration not attached 2. EC certificate attached 3. Free sale certificate not attached	Rejected
----	--	----------------------------	------------------------	--	--	----------

Authority letter from manufacturer not notarized attached

Authority letter from manufacturer not notarized attached

Authority letter from manufacturer not notarized attached



**M/s Hope Pharma & Distributors**

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks	
79	Glide Wire 0.035 (Ordinary) Straight / curved Hydrophilic 150CM	Poseidon Glide Wire 150cm	SP Medical Denmark	<ol style="list-style-type: none"> <li>No experience with this institute</li> <li>No experience with this institute</li> <li>Authority letter from manufacturer not notarized attached</li> </ol>	<ol style="list-style-type: none"> <li>End User Reservation</li> <li>Authority letter from manufacturer notarized attached</li> </ol>	<ol style="list-style-type: none"> <li>Invalid drug registration certificate attached</li> <li>Invalid drug registration certificate attached</li> </ol>	Rejected
80	Glide Wire Exchange Length 0.035 & 0.025 260CM Hydrophilic (Straight / Curved)	Poseidon Glide Wire 0.035 x 260 cm	SP Medical Denmark	<ol style="list-style-type: none"> <li>No experience with this institute</li> <li>Authority letter from manufacturer not notarized attached</li> </ol>	<ol style="list-style-type: none"> <li>End User Reservation</li> <li>Authority letter from manufacturer notarized attached</li> </ol>	Rejected	
34	PTCA GUIDE WIRE, WORK HORSE WIRE SOFT TIP, MODERATE SUPPORT, 0.014 AND 175-195 CM	Borer	MedasInc, USA	<ol style="list-style-type: none"> <li>No Cardiac Institute experience</li> <li>On license to import address different while on Drug Sale License address different and on FBR also different</li> <li>On Medical device registration brand name Borer while on technical offer it is Borer mentioned</li> <li>On Free sale certificate also Borer mentioned</li> <li>Authority letter from manufacturer not notarized attached</li> </ol>	<ol style="list-style-type: none"> <li>The Grievance committee evaluated the experience letters in detail. There were only two experiences of govt. teaching hospitals while others were from private hospitals that do not meet the bidding criteria. No cardiac institute experience (End User Reservation)</li> <li>On license to import address different while on Drug Sale License address different and on FBR also different</li> <li>MDR with name Borer provided</li> </ol>	Rejected	

4. FSL with the name Borer as mentioned on technical offer and MDR provided

As per my observation  
notified attached

M/s Ali Medical Store

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
67	TAPE FOR SKIN HYPOALLERGIC ADHESIVE (TRANSPARENT) 3X10 YARDS	Transplas	Slipha Pvt. Ltd. U	Poor Sticking	End User reservation	Rejected

M/s Husnain Pharma




Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
45	DISPOSABLE LATEX GLOVES FOR EXAMINATION ALL SIZES (BOX OF 100)	SAFEHAND	Top Glove SDN. BHD. Malaysia	1. Free sale certificate not attached 2. EC certificate not attached	1. Free sale certificate not attached 2. EC certificate not attached	Rejected
46	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 6	PROFEEL	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
47	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDERED) NO. 6	COMFIT	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
48	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 6.5	PROFEEL	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
49	DISPOSABLE	COMFIT	WRP Asia Pacific	Invalid Free sale certificate attached		Rejected

*(Handwritten signatures and initials)*

	LATEX SURGICAL GLOVES STERILIZED (POWDERED) NO. 65	PROFEEL	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	
50	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 7	PROFEEL	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
51	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDERED) NO. 7	COMFIT	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
52	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 7.5	PROFEEL	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected
53	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED ((POWDERED) NO. 7.5	COMFIT	WRP Asia Pacific SdnBhd Malaysia	Invalid Free sale certificate attached	Invalid Free sale certificate attached	Rejected

**M/s Ibrahim Enterprises**

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
45	DISPOSABLE LATEX GLOVES FOR EXAMINATION ALL SIZES (BOX OF 100)	QC	Sri Tarang, Thailand	1. License to import not attached 2. Invalid EC certificate attached	1. License to import attached 2. Invalid EC certificate attached	Rejected
63	PRICKERS (BLOOD LENCET)	RECO	HuailanTianda Medical, China	1. Invalid Free sale certificate attached 2. Invalid EC certificate attached	1. Valid Free sale certificate attached 2. Valid EC certificate attached	Accepted
68	THREE WAY STOP	SAFEONT	Silver Surgical	Poor Quality	End User Reservation	Rejected

COCK -  
STANDARD

Complex PAK

M/s Maz International

Bid

Sr	Company Name	TAC Observations	GC Observation	Remarks
1	Bid Reject of M/s Maz International	1. Punjab govt. teaching institute experience not attached	1. Punjab govt. teaching institute experience not attached	Rejected

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
45	DISPOSABLE LATEX GLOVES FOR EXAMINATION ALL SIZES (BOX OF 100)	Sempermed	Sempermed Asia Pte.Ltd, Malaysia	<p>1. Invalid Free sale certificate attached</p> <p>2. License to import from Hope Pharma not attached</p> <p>3. On technical offer country of origin / manufacturer name Sempermed Asia Malaysia mentioned while on authority letter / free sale certificate it is Semperit Austria mentioned.</p> <p>4. Invalid EC certificate attached</p> <p>5. Authority letter from manufacturer to M/s Hope Pharma not notarized attached</p>	<p>1. Valid Free sale certificate attached</p> <p>2. License to import from Hope Pharma attached</p> <p>3. Authority letter / free sale certificate from Sempermed Asia Malaysia not provided</p> <p>4. Invalid EC certificate attached</p> <p>5. Authority letter from manufacturer to M/s Hope Pharma not notarized attached</p>	Rejected

M/s Medtronic Pakistan Pvt Limited

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
28	PERMANENT PACEMAKER SINGLE CHAMBER (INTRODUCER SHEATH + LEAD+BATTERY) VVIR	SPSR01/IPG SPHERA SR MRI SURESCAN, SPHERA	Medtronic Singapore/Switzerland/USA	1. Free sale certificate not attached 2. FDA certificate not attached	1. Free sale certificate attached 2. FDA certificate attached	Accepted
30	PTCA BALLOON MONORAIL NON-COMPLIANT-ALL SIZES	NC Euphora	Medtronic Mexico/USA	1. Free sale certificate not attached 2. FDA certificate not attached	1. Free sale certificate attached 2. FDA certificate attached	Accepted
31	PTCA BALLOON MONORAIL (SEMI COMPLIANT) - ALL SIZES	Sprinter Legend	Medtronic Mexico/USA	FDA/ EC certificate not attached	FDA certificate attached	Accepted
34	PTCA GUIDE WIRE, WORK HORSE WIRE SOFT TIP, MODERATE SUPPORT, 0.014 AND 175-195 CM	Cougarxt	Medtronic USA	1. FDA/ EC certificate not attached 2. Free sale certificate not attached 3. Not suitable work horse wire	1. FDA certificate attached 2. Free sale certificate not attached 3. End User Reservation	Rejected

M/s Safeway Systems Pakistan

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
19	INFLATION DEVICE WITH (Y-CONNECTOR)	KDL	China	1. Authority letter not attached	1. Authority letter provided	Accepted

*[Handwritten signatures and initials]*

(INTRODUCER  
NEEDLE)  
(TORQUER)

29 PRESSURE  
TUBING FOR  
HEMO DYNAMIC  
MONITORING

KDL

China

- 2. EC certificate not attached
- 3. Free sale certificate not attached
- 1. Sample not provided

- 2. EC certificate attached
- 3. Free sale certificate attached
- 1. Sample not provided

- 2. Punjab Teaching Govt. Institutes experience not attached
- 3. No experience with this institute
- 4. Authority letter not attached

- 2. Punjab Teaching Govt. Institutes experience not attached
- 3. End user reservation
- 4. Authority letter provided

Rejected

- 5. Free sale certificate not attached
- 6. EC certificate not attached

- 5. Free sale certificate attached
- 6. EC certificate attached

30 PTCA BALLOON  
MONORAIL NON-  
COMPLIANT-ALL  
SIZES

Medco

China

- 1. Sample not provided

- 1. Sample not provided

- 2. Punjab Teaching Govt. Institutes experience not attached
- 3. No experience with this institute
- 4. Authority letter not attached

- 2. Punjab Teaching Govt. Institutes experience not attached
- 3. End user reservation
- 4. Authority letter provided

Rejected

- 5. Medical device registration not attached
- 6. Free sale certificate not attached

- 6. Free sale certificate attached

62 MANOMETER  
LINE-200CM LONG

Welcare

Welford Medical M  
SDN BHD,  
Malaysia

- 1. Free sale certificate not attached
- 2. EC certificate not attached

- 1. Free sale certificate attached
- 2. EC certificate attached

Accepted

58 THREE WAY STOP

Welcare

Welford Medical M

- 1. Free sale certificate not attached

- 1. Free sale certificate attached

Accepted

COCK - STANDARD	SDN BHD, Malaysia	attached 2. EC certificate not attached	2. EC certificate attached
-----------------	-------------------	--	----------------------------

**The Searle Company Ltd**

**Bid**

Sr	Company Name	TAC Observations	GC Observation	Remarks
1	Bid Reject of M/s The Searle Company Ltd	1. Invalid DSL attached	1. Valid DSL attached	Accepted

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
48	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 6.5	Protix/TG Medical	Malaysia	Sufficient Punjab Teaching Govt. Institutes experience not attached	Sufficient Punjab Teaching Govt. Institutes experience attached	Accepted
49	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDERED) NO. 6.5	Protix/TG Medical	Malaysia	Sufficient Punjab Teaching Govt. Institutes experience not attached	Sufficient Punjab Teaching Govt. Institutes experience attached	Accepted
50	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDER FREE) NO. 7	Protix/TG Medical	Malaysia	Sufficient Punjab Teaching Govt. Institutes experience not attached	Sufficient Punjab Teaching Govt. Institutes experience not attached	Rejected
51	DISPOSABLE LATEX SURGICAL GLOVES STERILIZED (POWDERED) NO. 7	Protix/TG Medical	Malaysia	Sufficient Punjab Teaching Govt. Institutes experience not attached	Sufficient Punjab Teaching Govt. Institutes experience attached	Accepted
52	DISPOSABLE LATEX SURGICAL	Protix/TG Medical	Malaysia	Sufficient Punjab Teaching Govt. Institutes	Sufficient Punjab Teaching Govt. Institutes experience attached	Accepted



53	GLOVES STERILIZED (POWDER FREE) NO. 7.5	Protix/TG Medical	Malaysia	experience not attached Sufficient Punjab Teaching Govt. Institutes experience not attached	attached Sufficient Punjab Teaching Govt. Institutes experience not attached	Rejected
----	--	----------------------	----------	--	---	----------

**M/s TEK Enterprises**

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
33	PTCA GUIDE WIRE, HYDROPHILLIC, NON TAPERED STANDARD STRAIGHT TIP, MODERATE SUPPORT, POLYMER COATED 0.014 AND 175-195 CM	Fielder FC	Asahi Intec, Japan / Thailand	1. Authority letter from manufacturer not notarized attached 2. Free sale certificate not Embassy attested attached	1. Authority letter from manufacturer notarized attached 2. Free sale certificate Embassy attested attached	Accepted
34	PTCA GUIDE WIRE, WORK HORSE WIRE SOFT TIP, MODERATE SUPPORT, 0.014 AND 175-195 CM	Rinato	Asahi Intec, Japan / Thailand	1. Authority letter from manufacturer not notarized attached 2. Free sale certificate not Embassy attested attached	1. Authority letter from manufacturer notarized attached 2. Free sale certificate Embassy attested attached	Accepted
36	PTCA GUIDE WIRE, HYDROPHILLIC, TAPERED, INTERMEDIATE STRAIGHT TIP, MODERATE SUPPORT, POLYMER COATED, 0.014 AND 175-195 CM	Fielder XT	Asahi Intec, Japan / Thailand	1. Authority letter from manufacturer not notarized attached 2. Free sale certificate not Embassy attested attached	1. Authority letter from manufacturer notarized attached 2. Free sale certificate Embassy attested attached	Accepted
37	PTCA GUIDE	Grand Stream	Asahi Intec, Japan	1. Authority letter from	1. Authority letter from	Accepted

	WIRE, EXTRA SUPPORT WIRE, 0.014 AND 175-195 CM		/ Thailand	<p>manufacturer not notarized attached</p> <p>2. Free sale certificate not Embassy attested attached</p>	<p>manufacturer notarized attached</p> <p>2. Free sale certificate Embassy attested attached</p>	
38	CTO PCI GUIDE WIRES RADIO OPAQUE PART 15CM HYDROPHILIC COATING 40CM (I) TIP LOAD 1.5-2 GM	Gaia I	Asahi Intec, Japan / Thailand	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer not notarized attached</p> <p>3. Free sale certificate not Embassy attested attached</p>	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer notarized attached</p> <p>3. Free sale certificate Embassy attested attached</p>	Rejected
38	II. TIP LOAD 3.- 4.5 GM	Gaia II	Asahi Intec, Japan / Thailand	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer not notarized attached</p> <p>3. Free sale certificate not Embassy attested attached</p>	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer notarized attached</p> <p>3. Free sale certificate Embassy attested attached</p>	Rejected
38	III. TIP LOAD - 4.5 GM	Gaia III	Asahi Intec, Japan / Thailand	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer not notarized attached</p> <p>3. Free sale certificate not Embassy attested attached</p>	<p>1. Invalid EC certificate attached</p> <p>2. Authority letter from manufacturer notarized attached</p> <p>3. Free sale certificate Embassy attested attached</p>	Rejected

M/s Yousaf &amp; Co

Bid

Sr	Company Name	TAC Observations	GC Observation	Remarks
1	Bid Reject of M/s Yousaf & Co	2. Invalid DSL attached	2. Valid DSL attached	Accepted

Item #	Item Name	Brand Name	Manufactured by	TAC Observations	GC Observation	Remarks
45	Disposable latex Gloves for Examination all sizes	Primax Examination Gloves	Biomax Malaysia	<ol style="list-style-type: none"> <li>Authority letter from manufacturer not notarized attached</li> <li>EC certificate not attached</li> </ol>	<ol style="list-style-type: none"> <li>Authority letter from manufacturer attached</li> <li>EC certificate attached</li> </ol>	Accepted

**M/S Global Marketing Services Bid**

Sr	Company Name	TAC Observations	GC Observation	Remarks
1	Bid Reject of M/s Global Marketing Services	<ol style="list-style-type: none"> <li>Drug Sale license not attached</li> <li>Bid form not signed and stamped</li> </ol>	<ol style="list-style-type: none"> <li>Renewal slip for DSL attached</li> <li>Bid form signed and stamped attached</li> </ol>	Accepted

**M/S Alliance Medical**

Sr.	Description	Firm Grievance	GC Observation	Decision
1	Grievance Against M/s Ali medical Store	<p>The firm claims that</p> <ol style="list-style-type: none"> <li>Manometer line quoted by Ali Medical Store is a pressure line. The Bicakclar, turkey does not produce a product to meet with specifications of manometer line</li> <li>The product has been rejected by various hospitals</li> </ol>	<p>Manometer line and Pressure line both are extension lines used for same purpose. Manometer line length is 200 cm and pressure line is 800 cm.</p>	<p>Grievance of M/S Alliance medical rejected and product Pressure line of M/S Ali Medical store accepted.</p>
2	Grievance Against M/s Cardiac Care	<p>The firm claims that Manometer line quoted by M/S Cardiac care mentioned country of origin as Europe in its technical bid. As Europe is continent comprising of several-countries and it does not reflect particular country of origin. In this way, the bidder has deliberately attempted to conceal the information in documents. The registration certificate of manometer line of M/s Cardiac Care is attached in the bid.</p>	<p>Firm provided the affidavit</p>	<p>Grievance of M/S Alliance medical rejected and product Manometer line of M/S Cardiac Care accepted.</p>


AS FRANCE


**M/S A & E Medical**

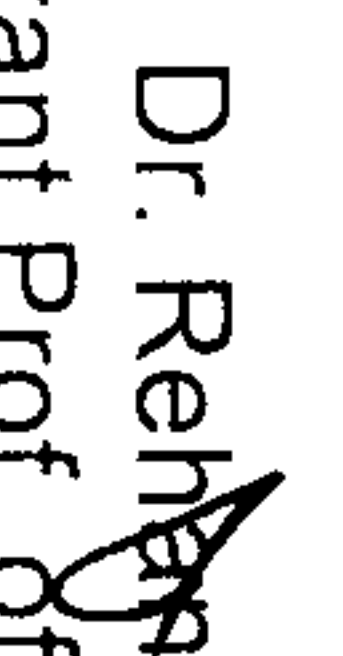
Sr.	Description	Firm Grievance	GC Observation	Decision
1	Grievance Against M/s Alliance medical	The firm claims that The TPM lead quoted by M/S Alliance Medical are not compatible with pacemaker and are of poor quality	The Product has been already Technically not approved	Grievance of M/S A & E Medical rejected

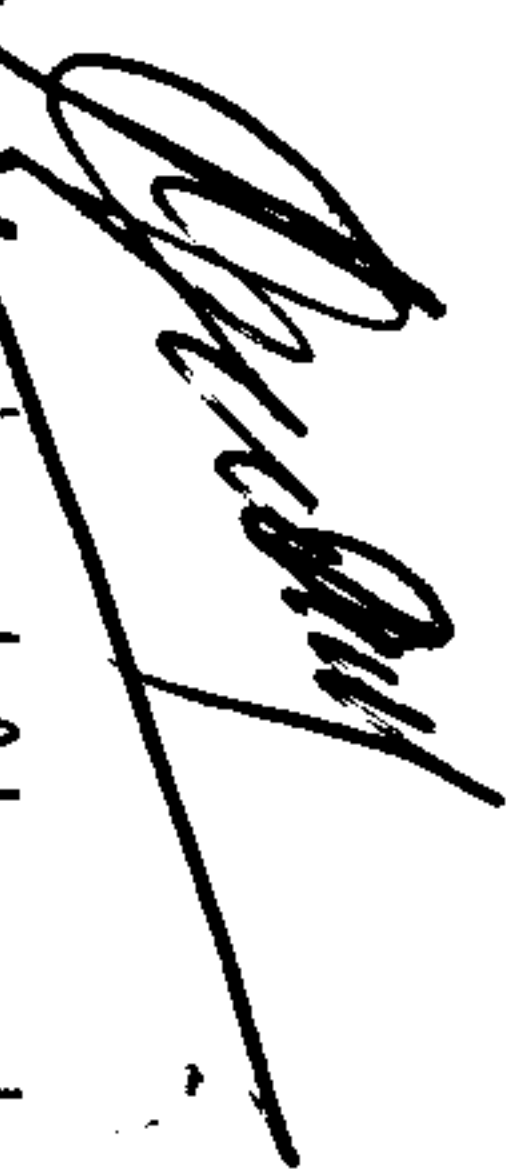
**Global Marketing Services**


Sr.	Description	Firm Grievance	GC Observation	Decision
1	Grievance Against M/s Atco	The registration provided by Alvimedica for Guiding Catheters is under Drug Rule and not Valid for medical devices	The Alvimedica provided MDR for Guiding catheters	Grievance of M/S Global Marketing Services rejected and product Guiding Catheters of M/S Atco accepted.

  
 Mrs. Iqra Munir,  
 Pharmacist,  
 FIC, Faisalabad.

  
 Engr. Sharaz Ali  
 Bio Medical Engineer  
 FIC, Faisalabad.

  
 Dr. Rehman Riaz  
 Assistant Prof. of Cardiology,  
 FIC, Faisalabad.

  
 Dr. Maqbool Ahmed,  
 PMO,  
 FIC, Faisalabad.

  
 Dr. Shahbaz Ahmad Khiliji,  
 Prof. of Cardiac Surgery,  
 FIC, Faisalabad